PATENT APPLICATION

25267

PATENT, TRADEMARK OFFICE

THE UNITED STATES PATENT AND TRADEMARK OFFICE

Group: 2632 }

Atty. Docket: 8266-0519 }

Applicants: Reeder et al. }

Invention: PATIENT POINT OF CARE }


Serial No.: 09/849,580 }

Filed: May 4, 2001 }

Examiner: Unknown }

Certificate Under 37 CFR 1.8(a)

I hereby certify that this correspondence is being deposited with the United States Postal Service with sufficient postage for first class mail in an envelope addressed to Box Issue Fee, Assistant Commissioner for Patents, Washington, D.C. 20231

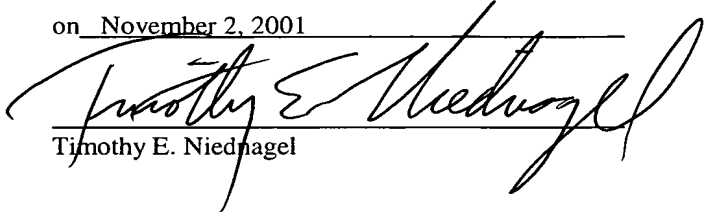on November 2, 2001

 Timothy E. Niednagel
LETTER TO OFFICIAL DRAFTSMAN

Box Missing Parts
Commissioner for Patents
Washington, D.C. 20231


Dear Sir:

Applicants submit herewith formal drawings for the above-identified application meeting the requirements of 37 CFR Section 1.84.

If the Draftsman has any questions regarding the drawings, please contact applicants' undersigned attorney, at (317) 684-5251.

Respectfully submitted,

BOSE McKINNEY & EVANS LLP

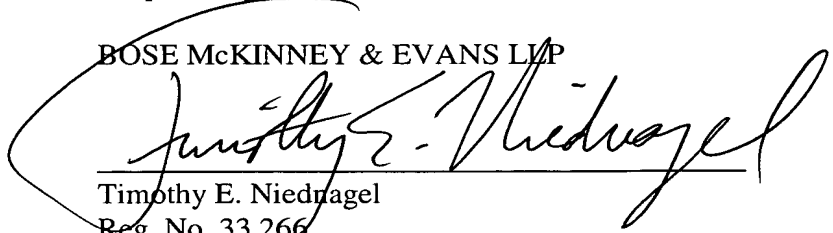
 Timothy E. Niednagel
 Reg. No. 33,266

TEN:kyb
Indianapolis, Indiana
(317) 684-5251
::ODMA\MHODMA\DT1;268510;1

09849580-121801

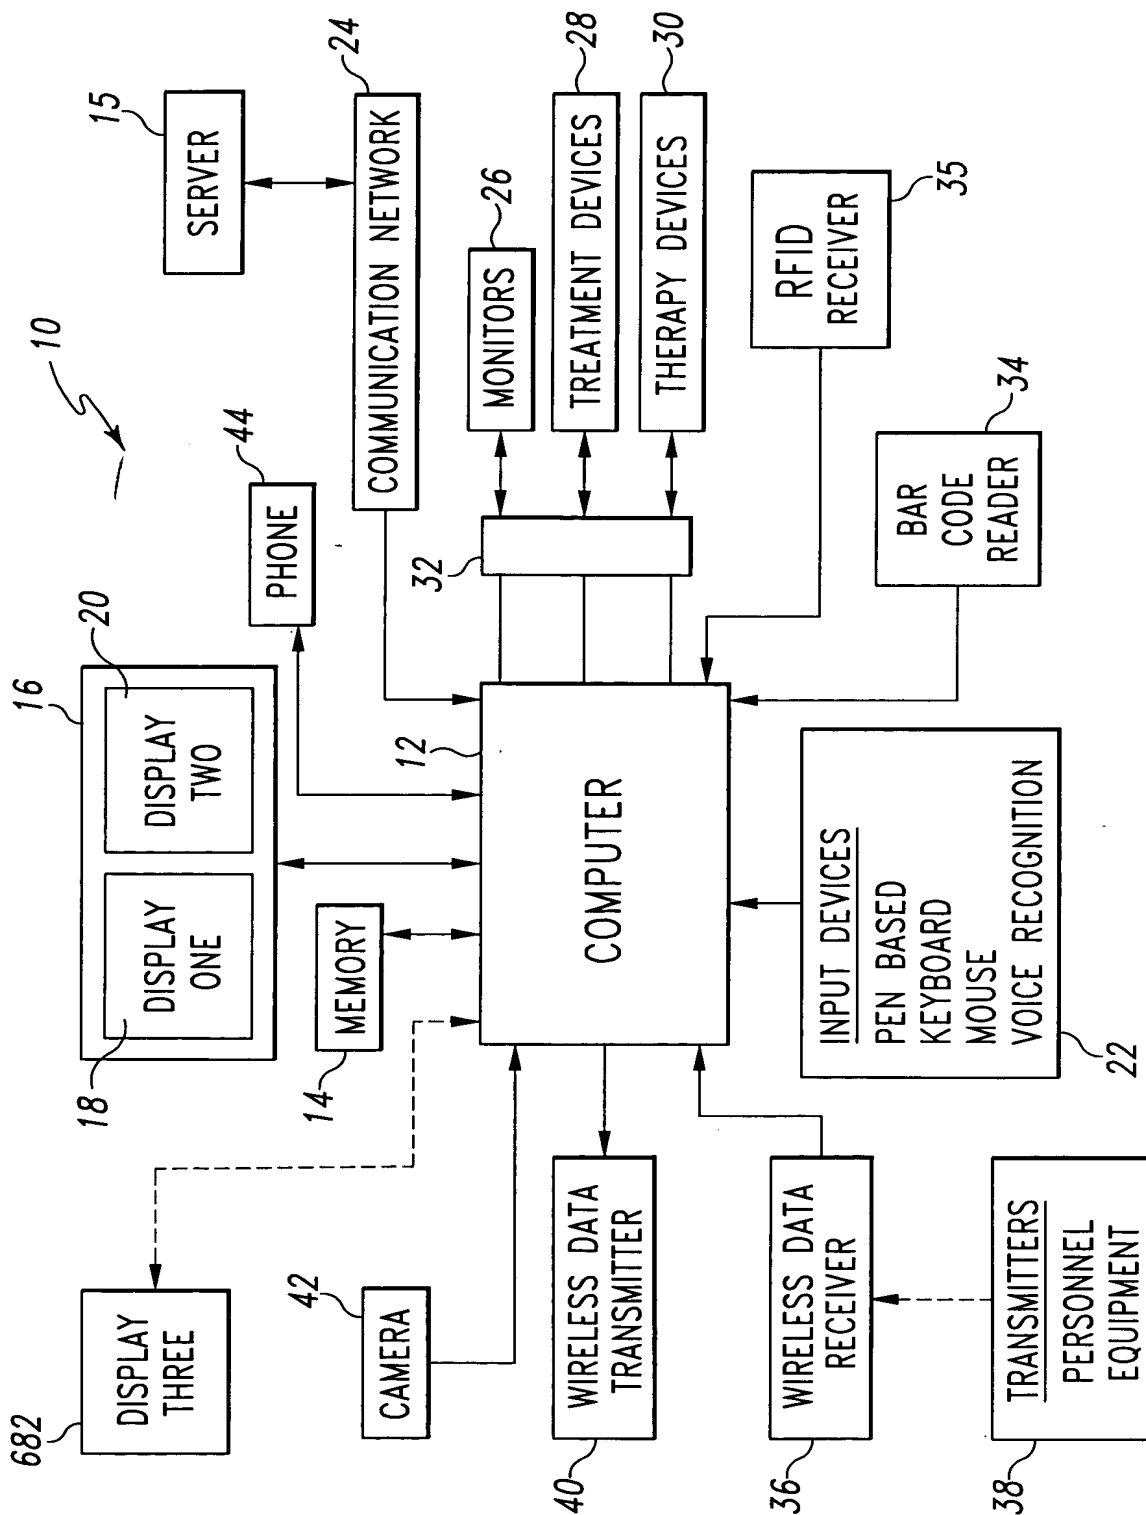


Fig. 1

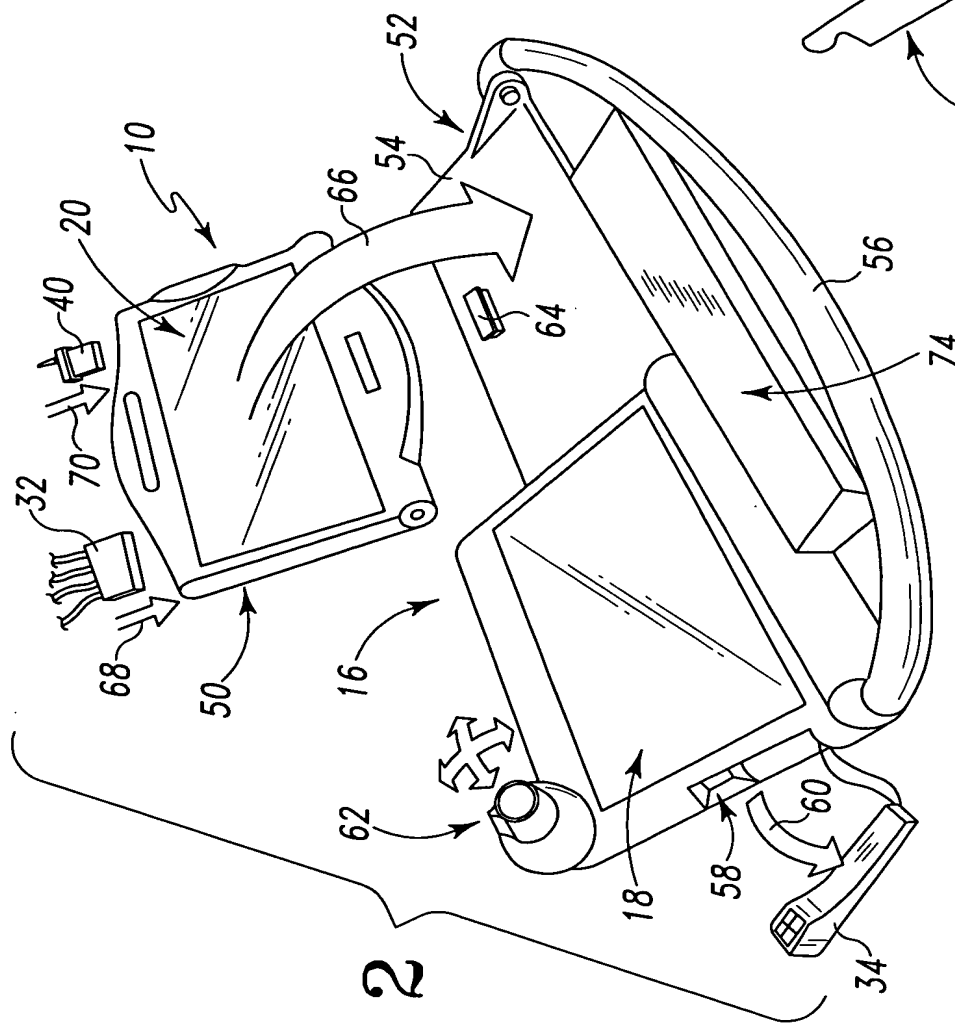


Fig. 2

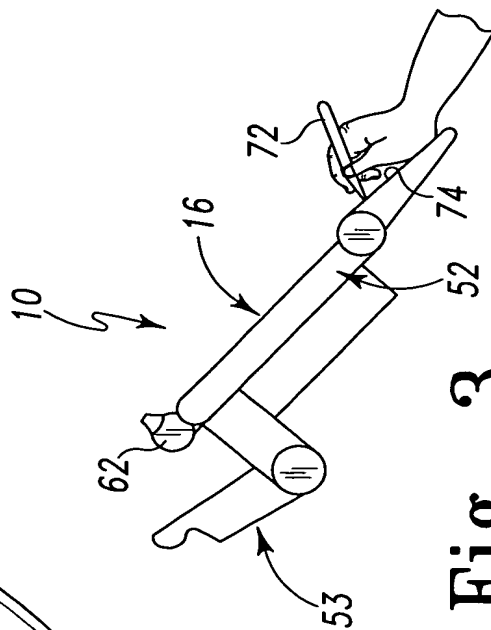


Fig. 3

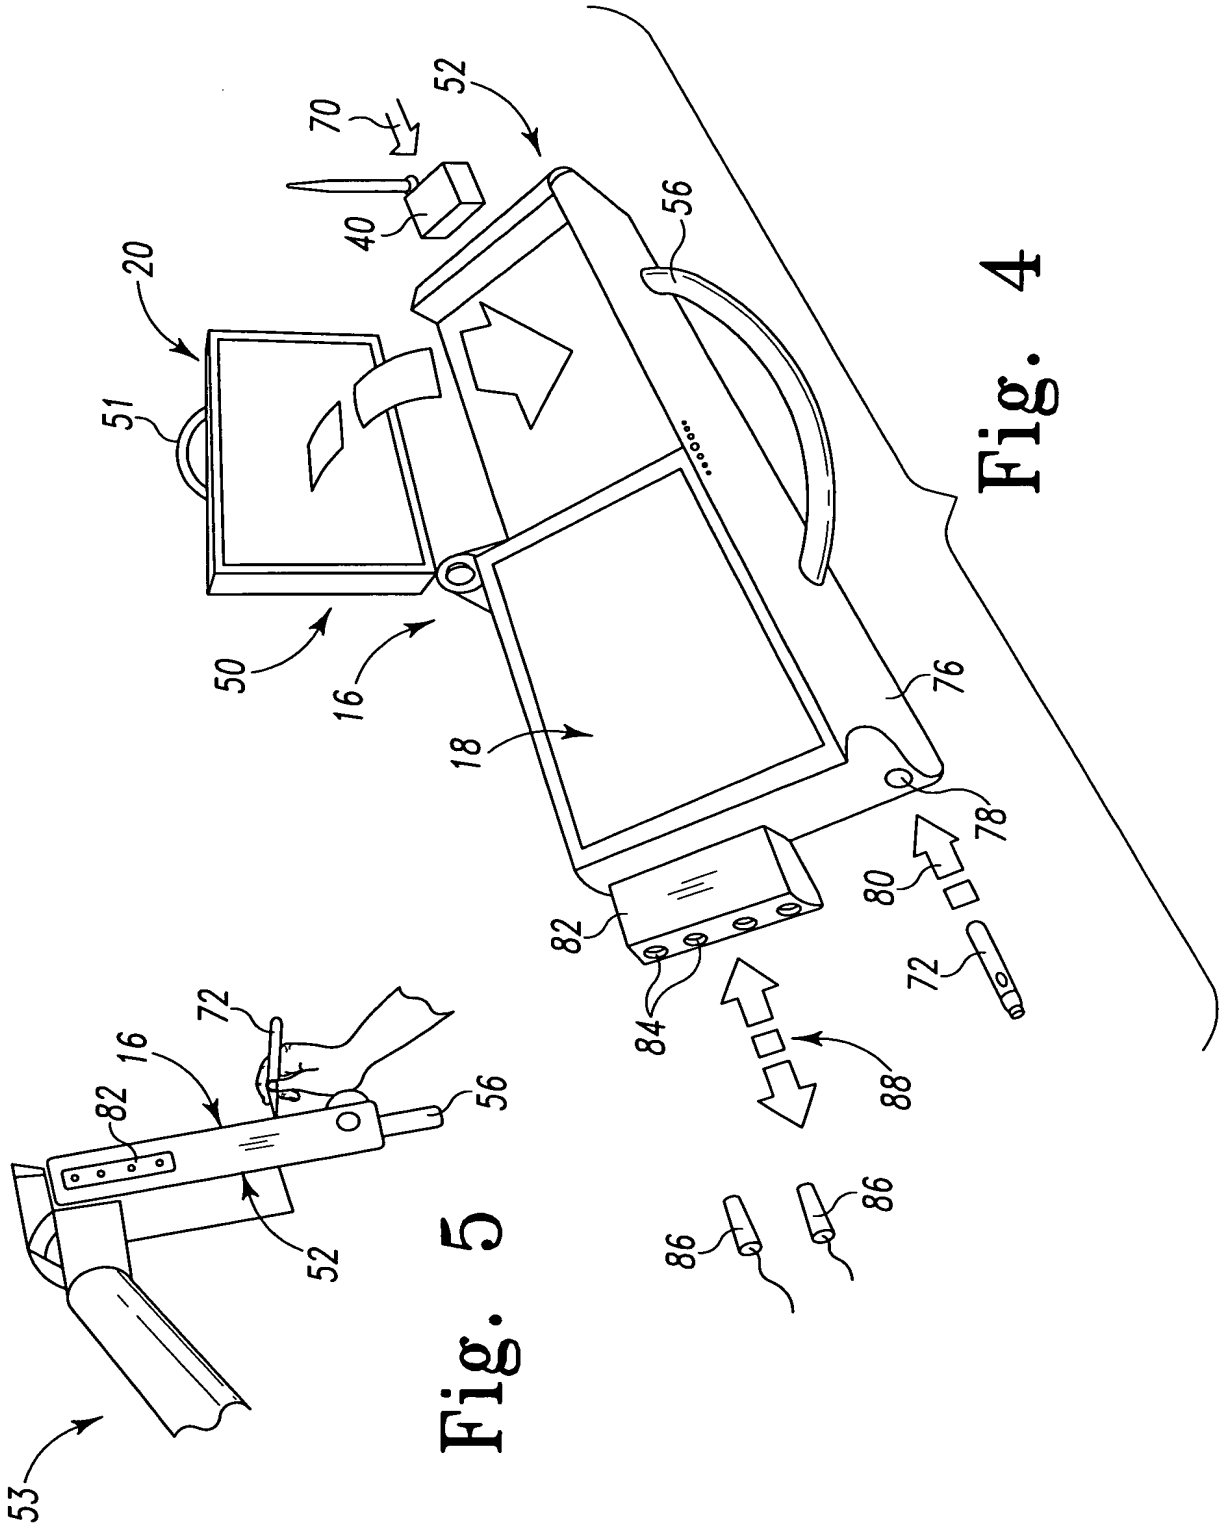


Fig. 5

Fig. 4

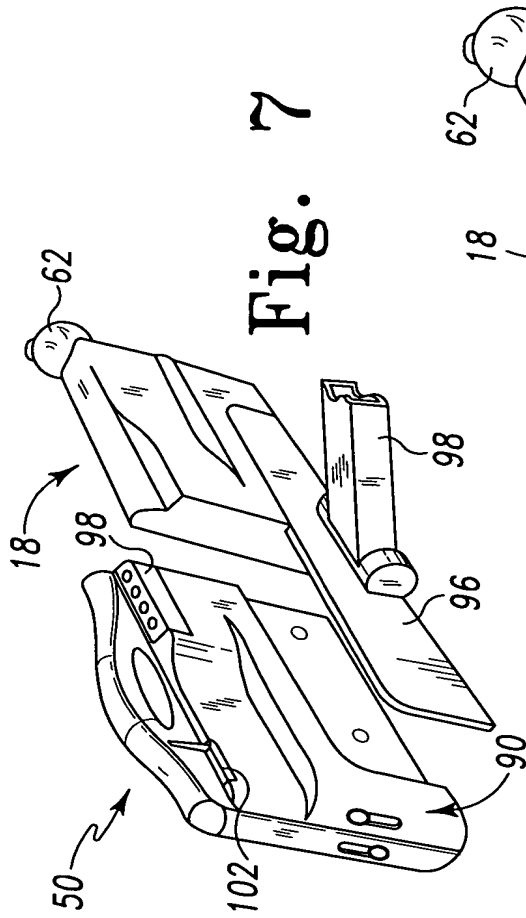


Fig. 7

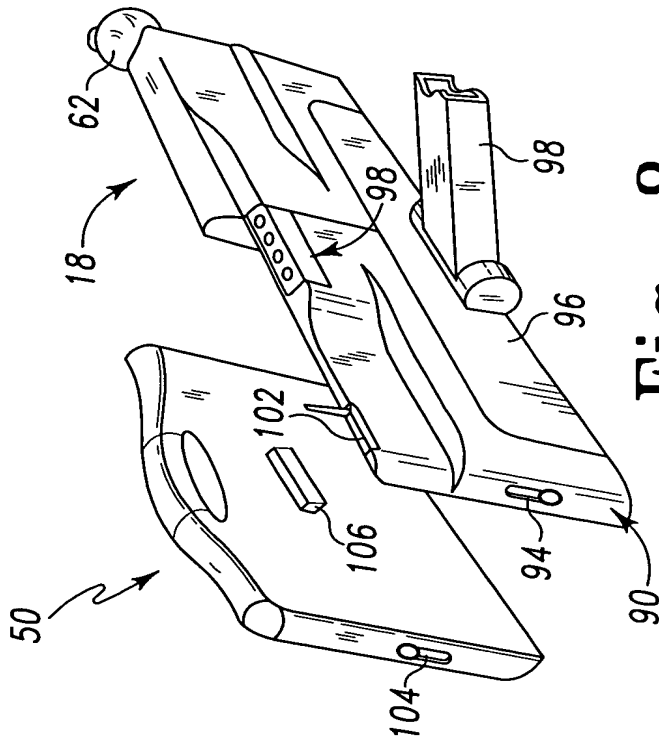


Fig. 8

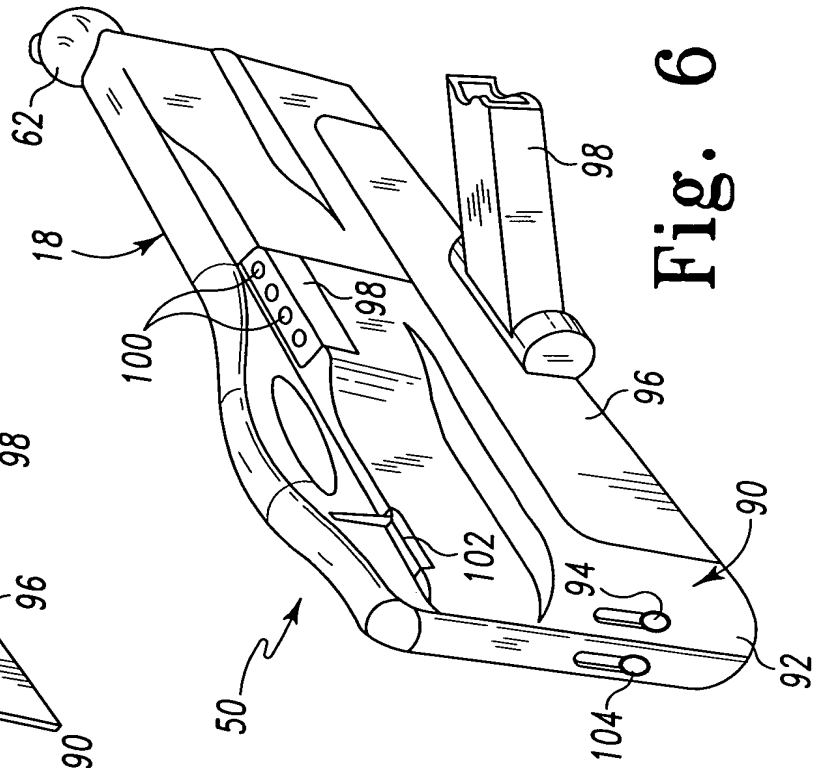


Fig. 6

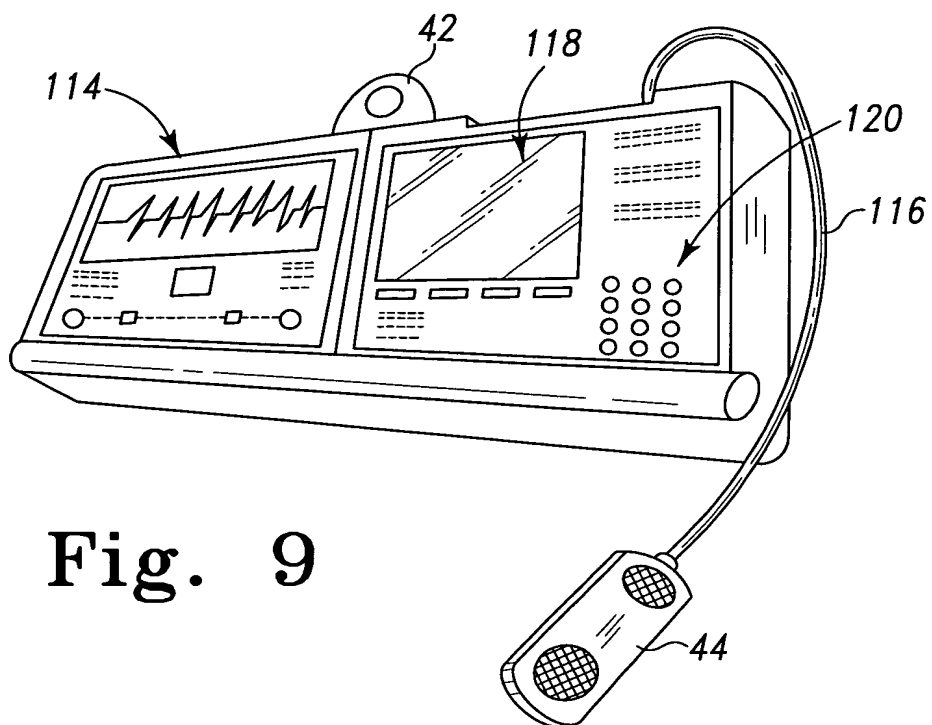


Fig. 9

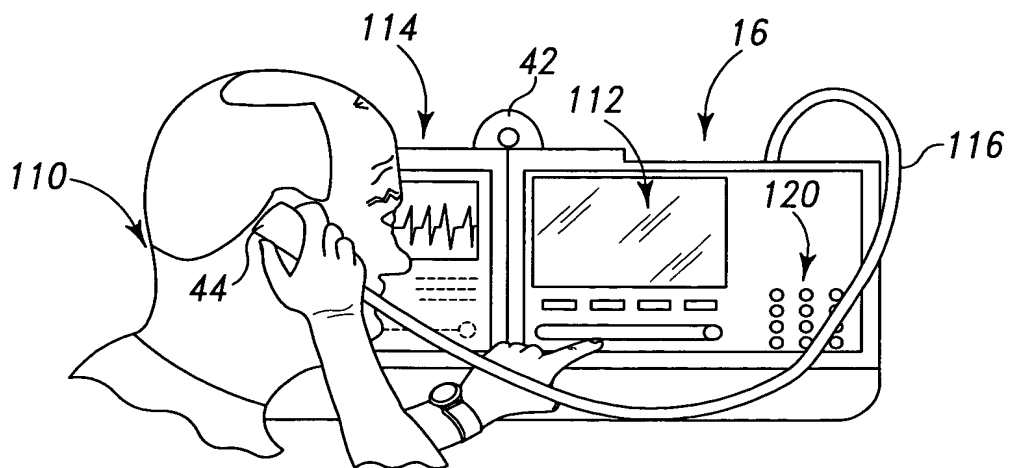


Fig. 10



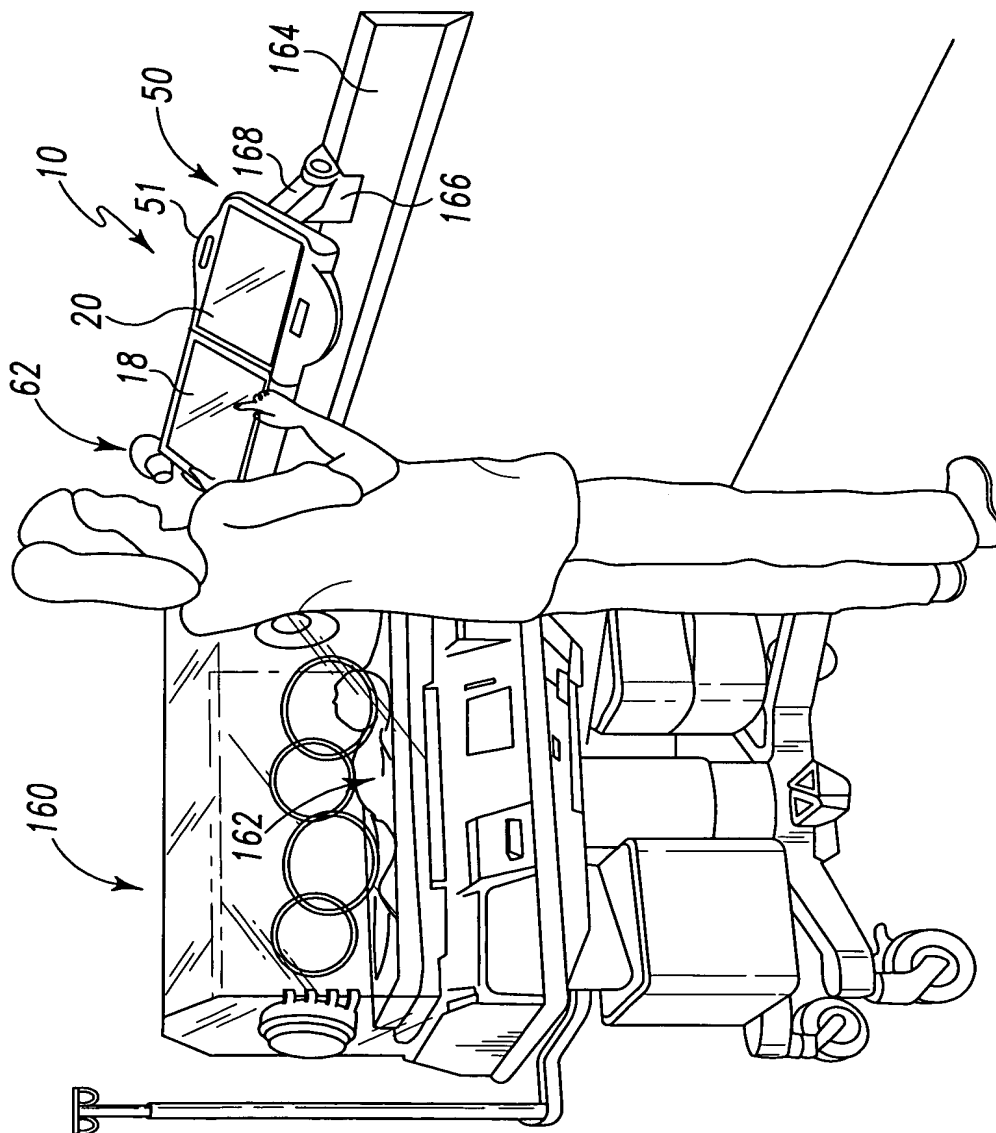


Fig. 12



9/59

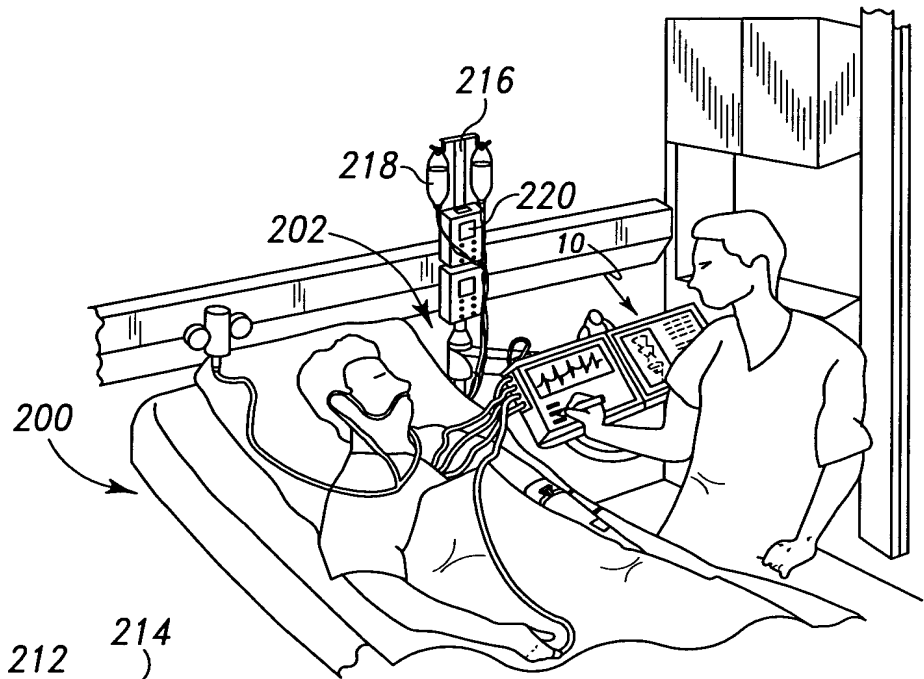


Fig. 15

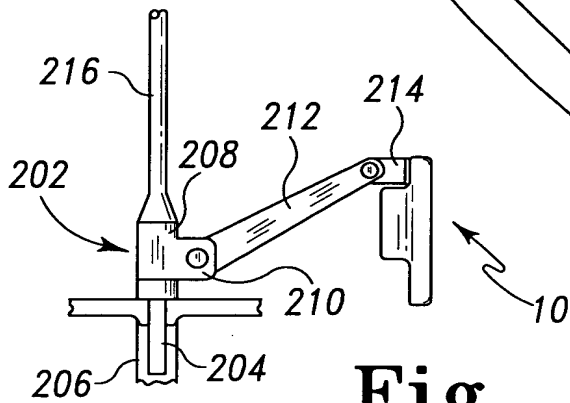


Fig. 16

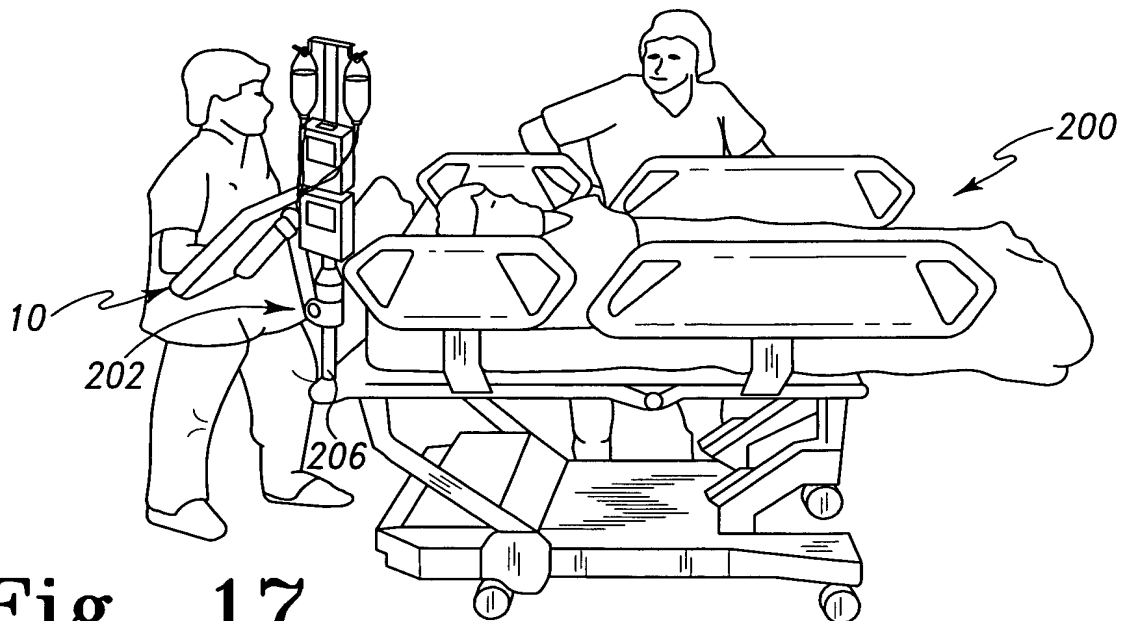


Fig. 17

09549580-121801

10/59

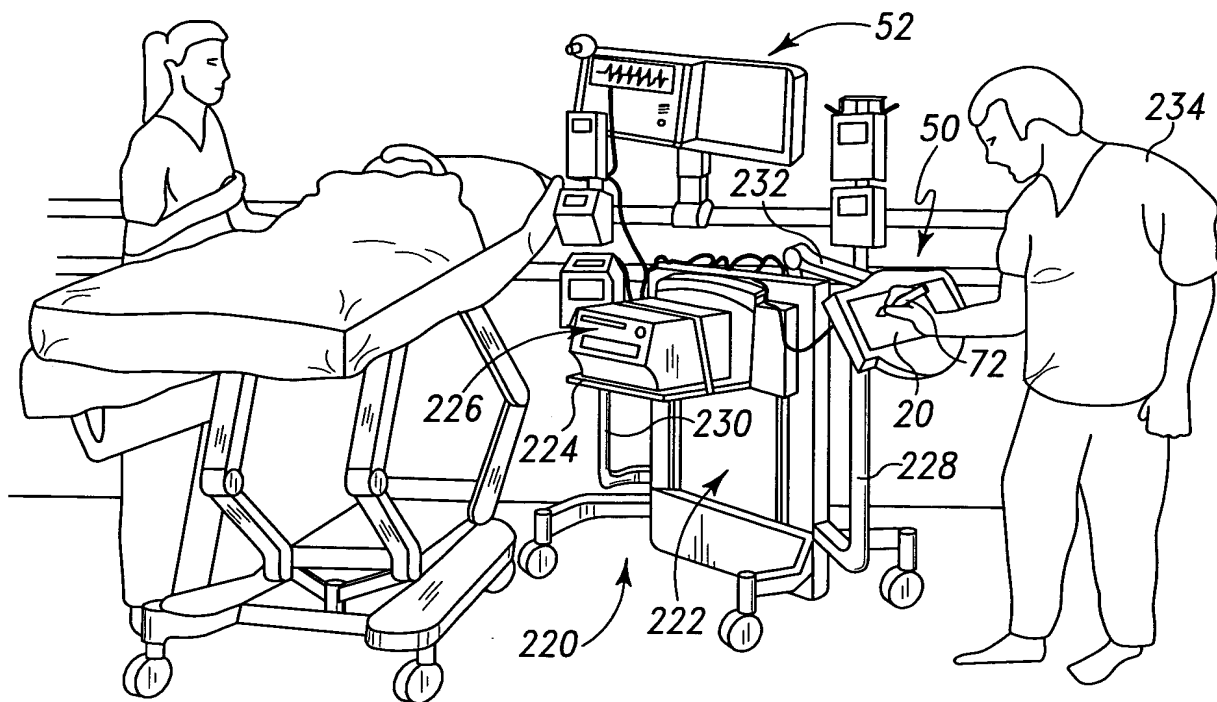


Fig. 18

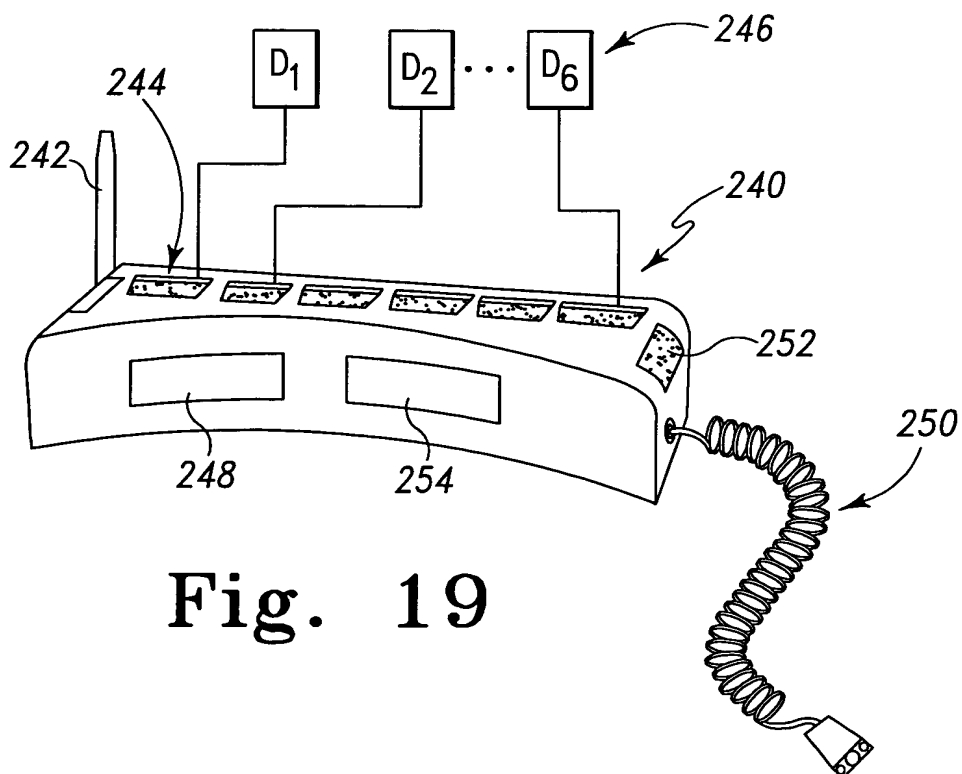


Fig. 19

09519580-121301

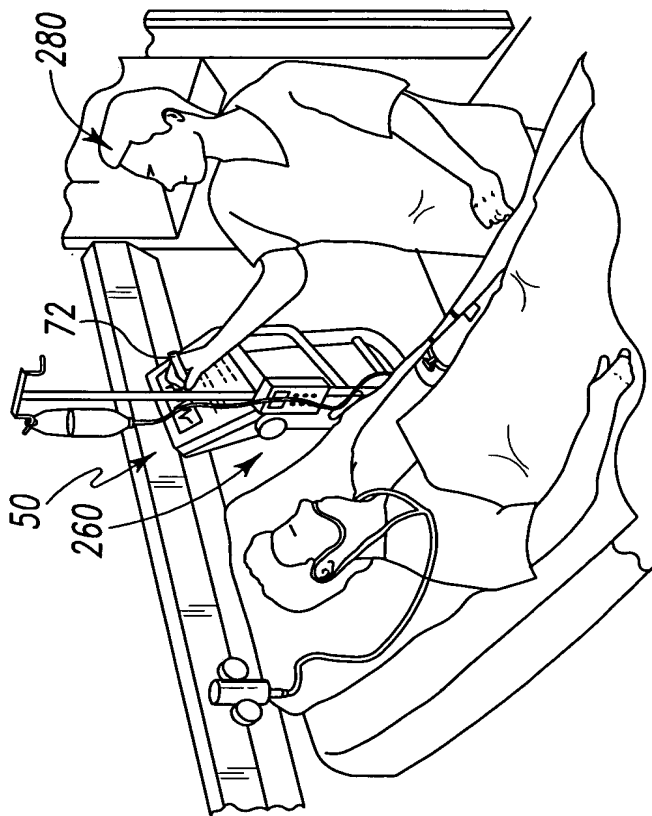


Fig. 21

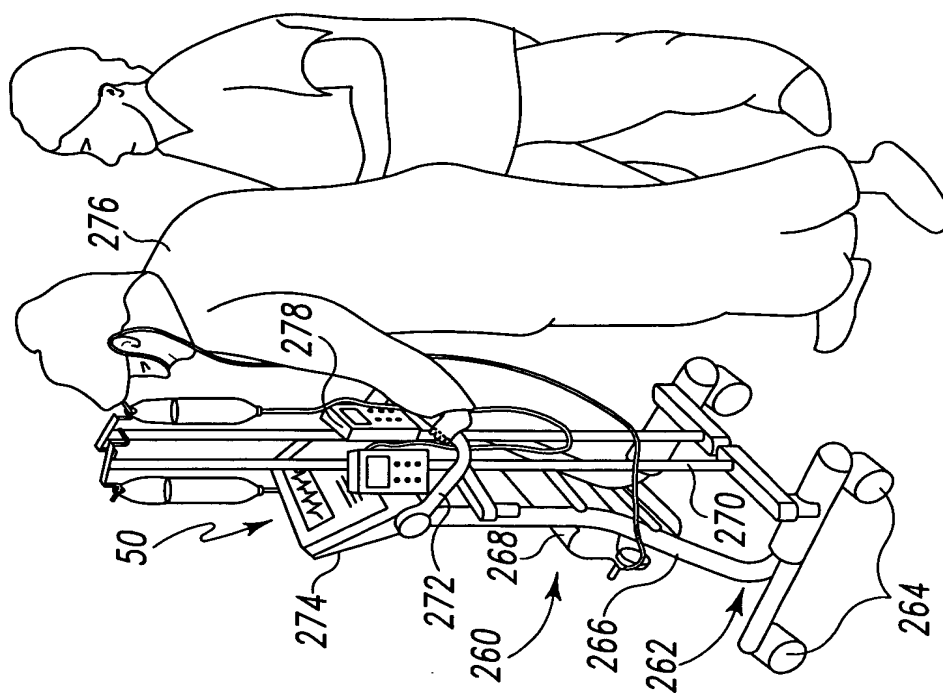


Fig. 20

12/59

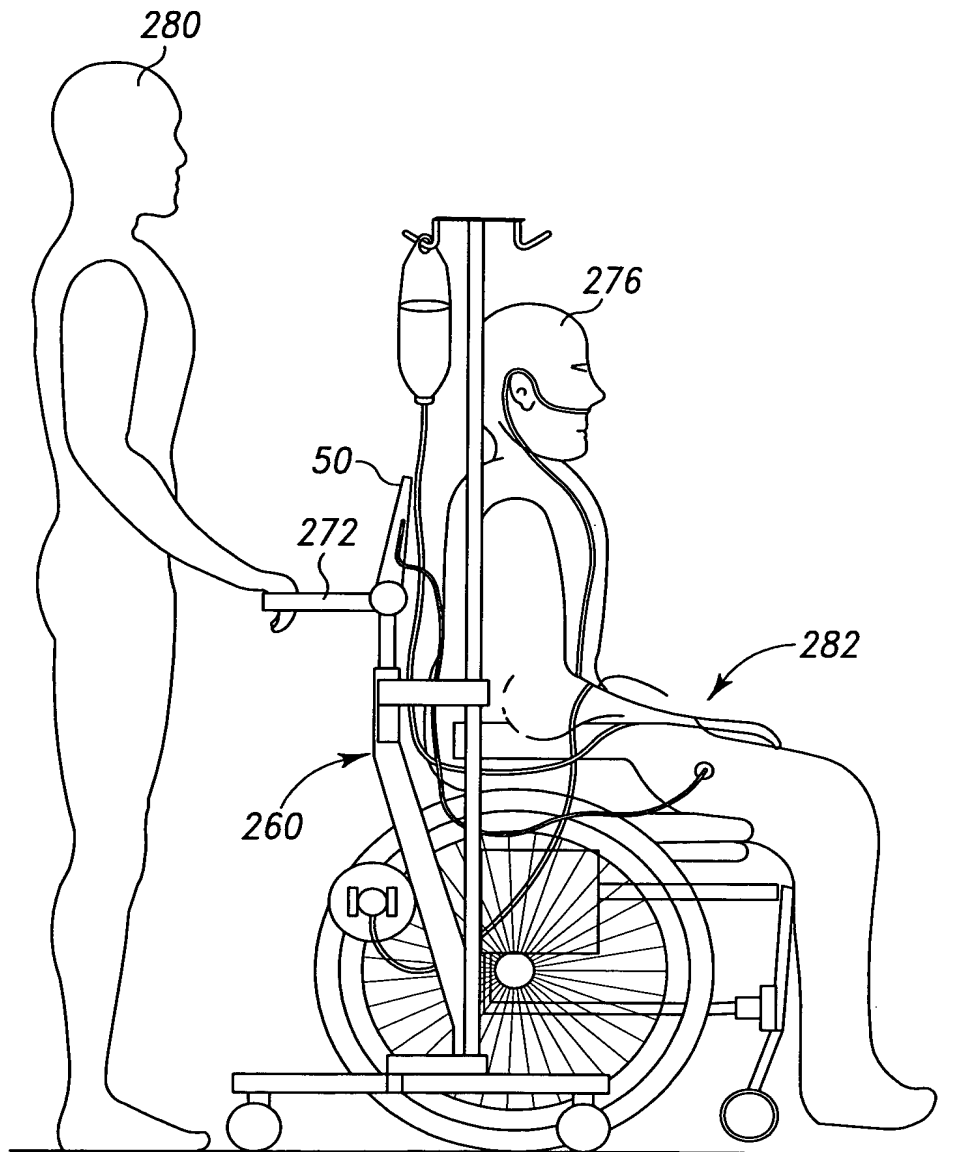


Fig. 22

09849580-121801

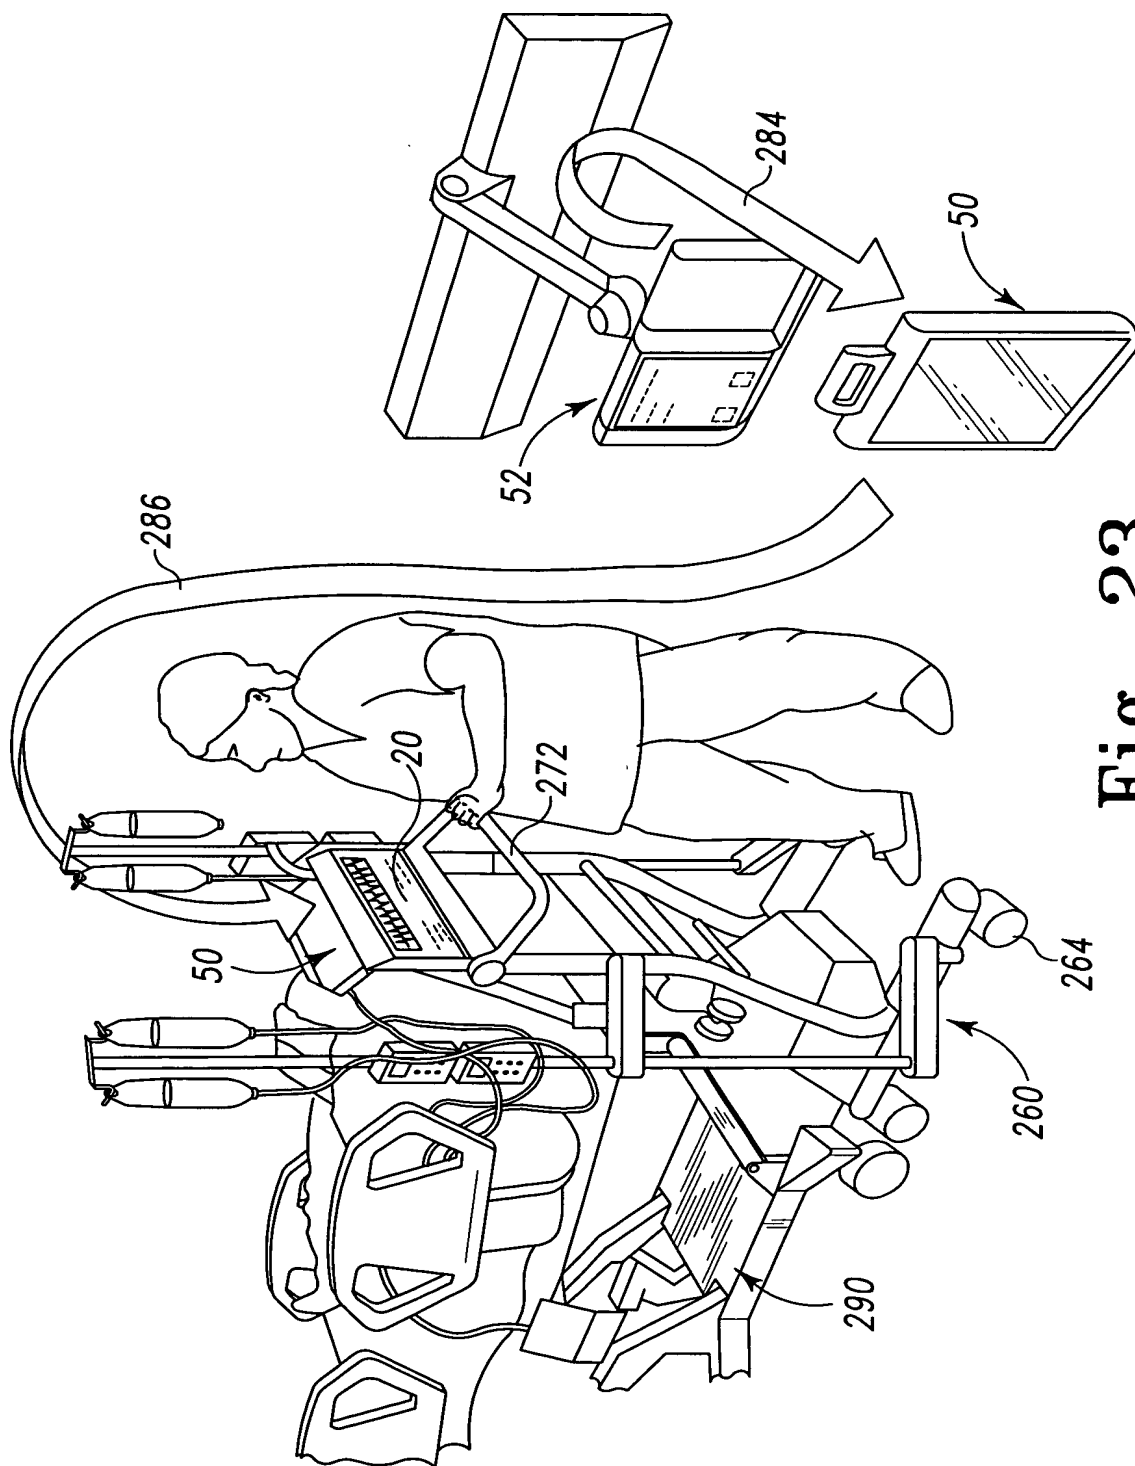


Fig. 23

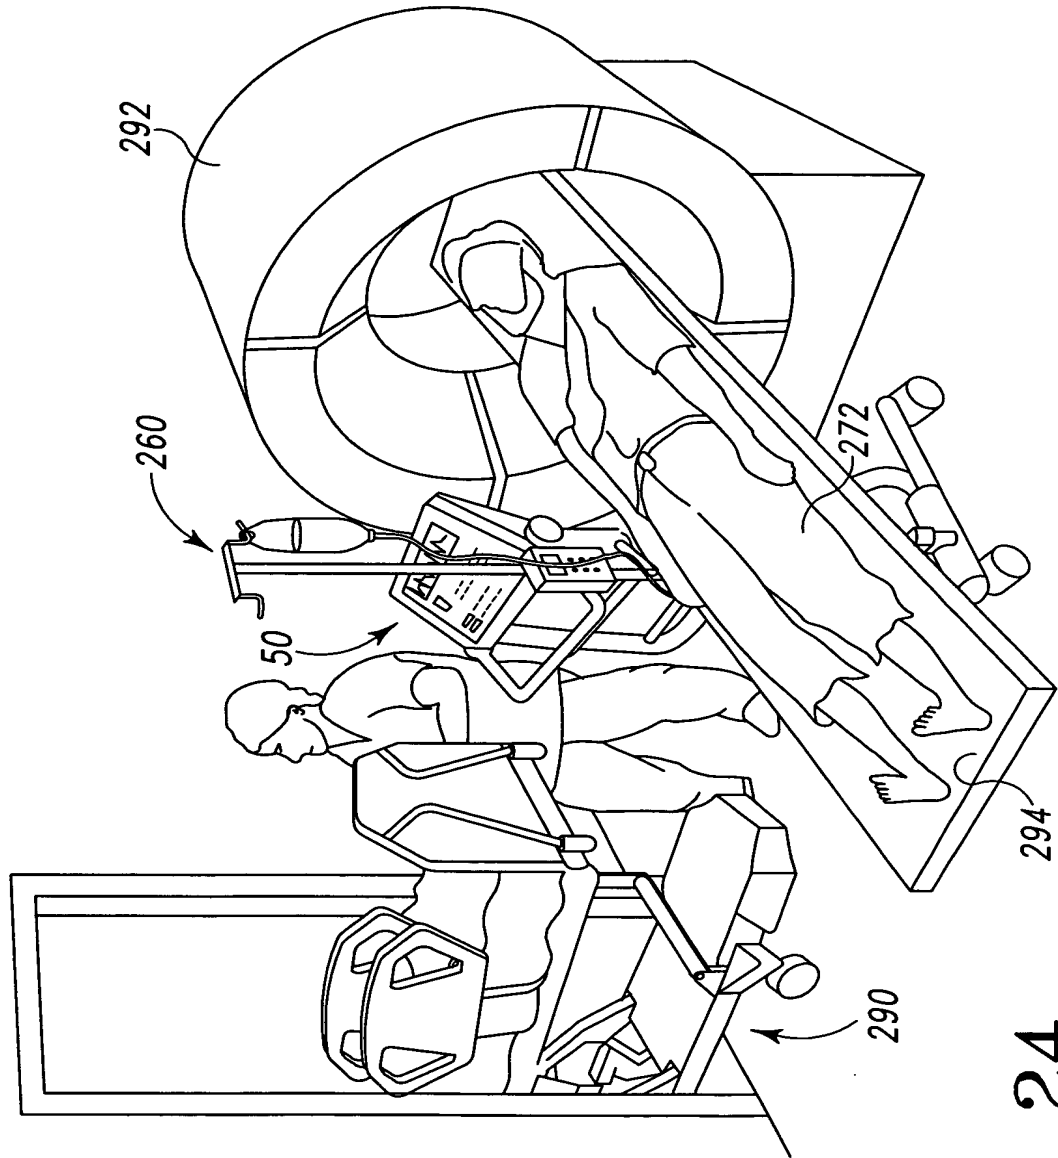


Fig. 24

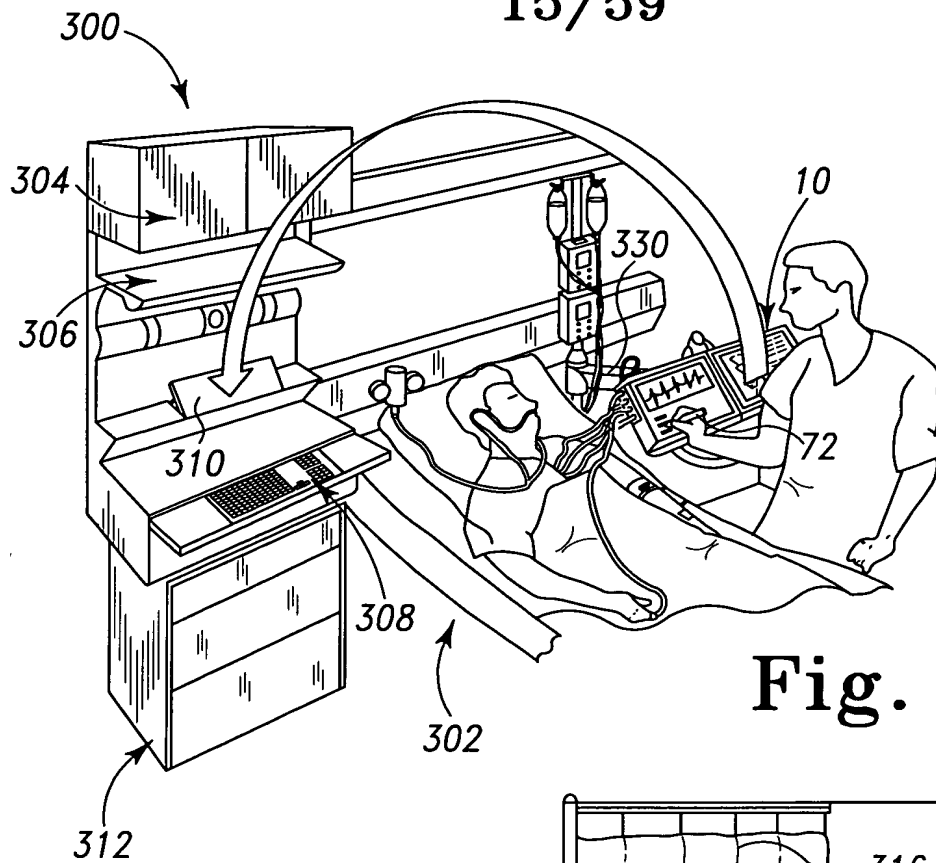


Fig. 25

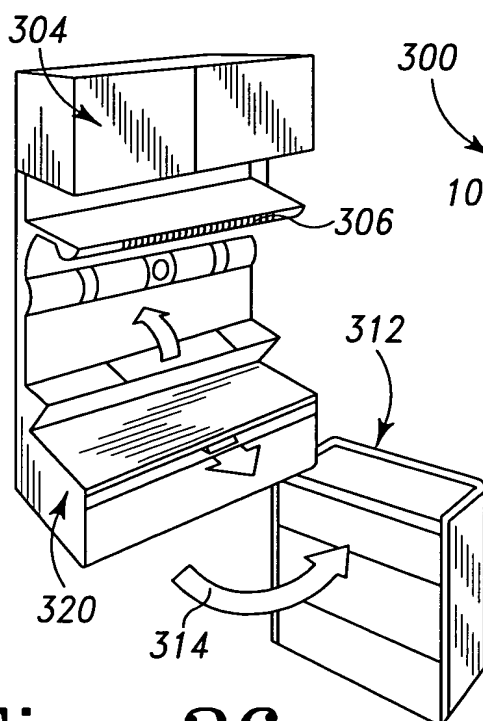


Fig. 26

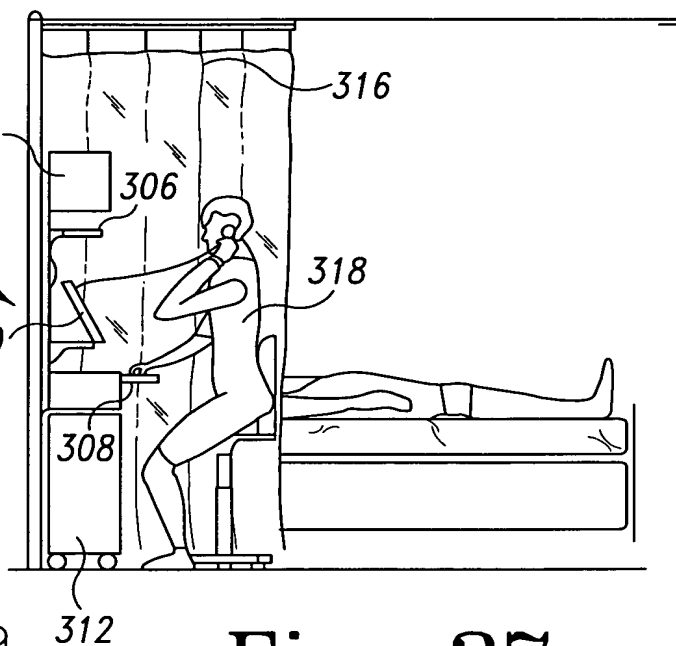


Fig. 27

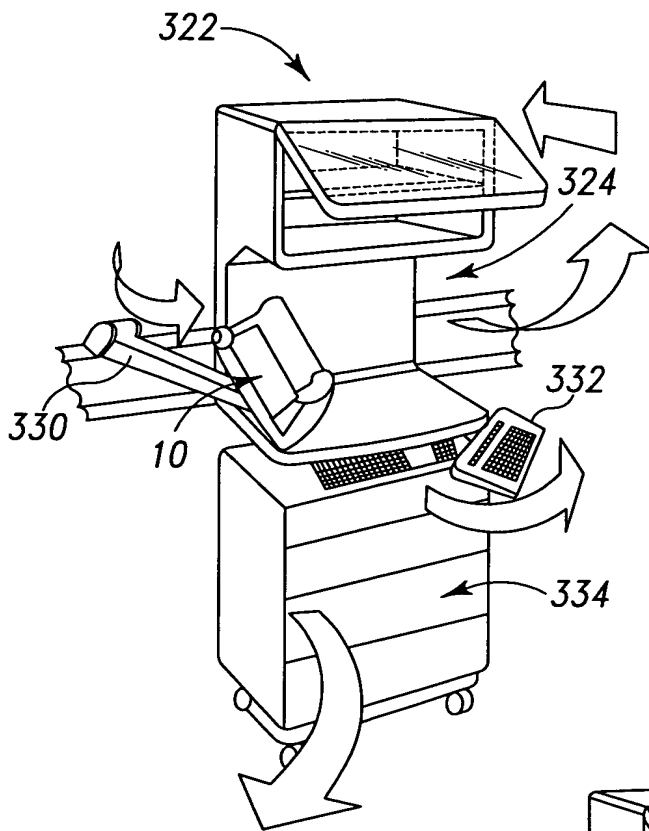


Fig. 29

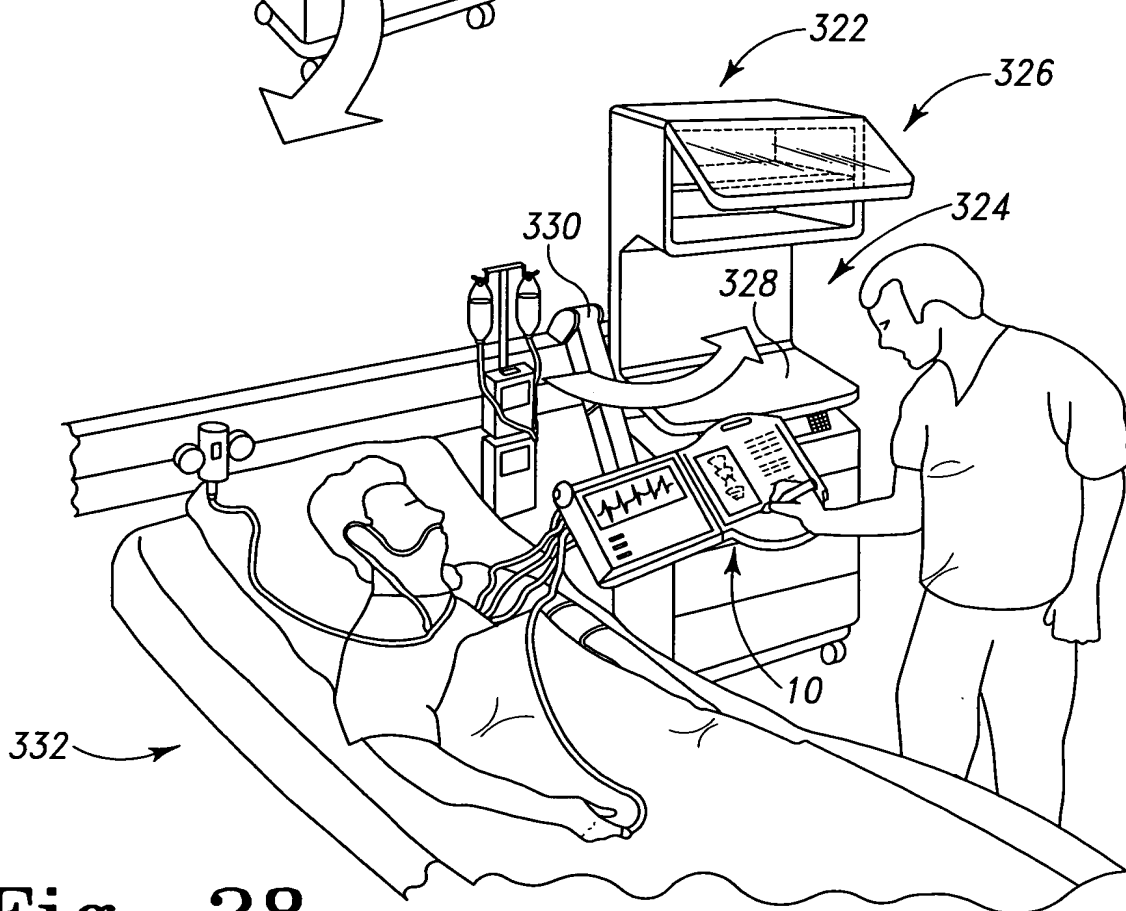


Fig. 28

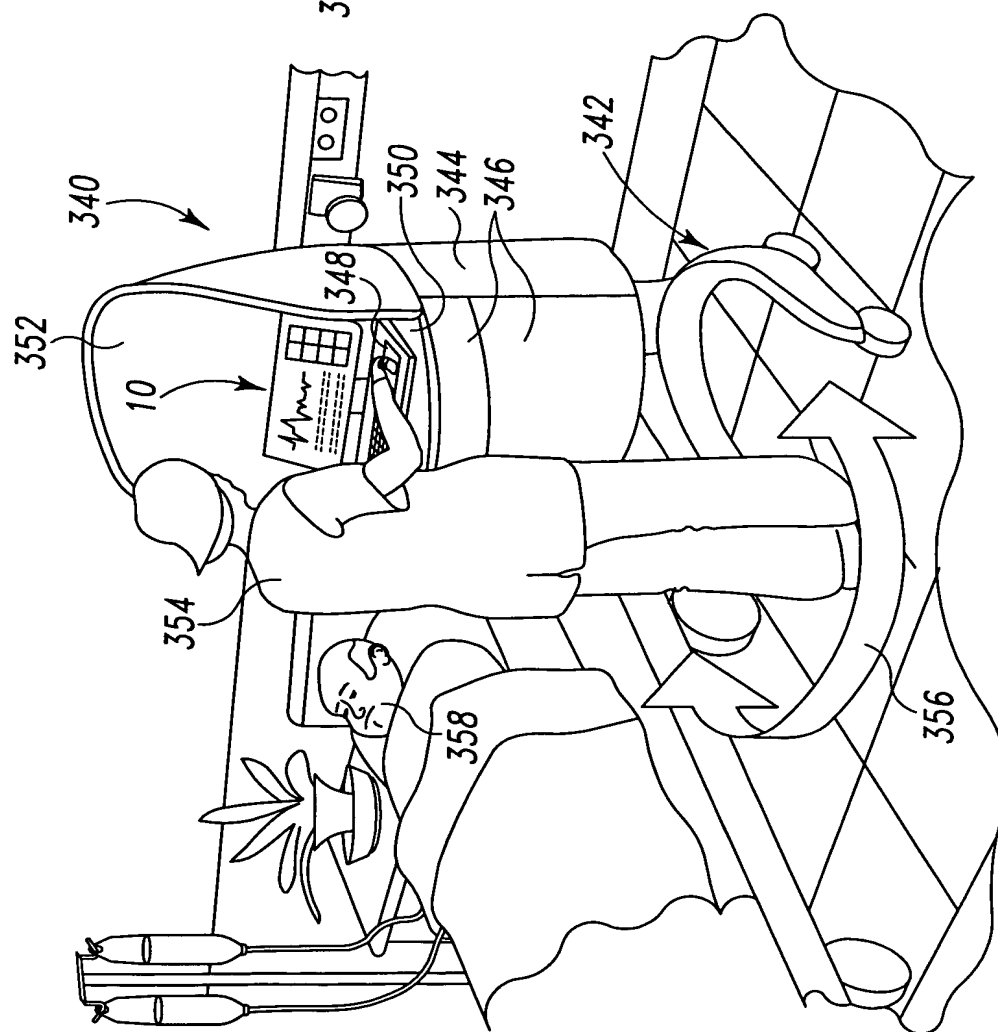


Fig. 30

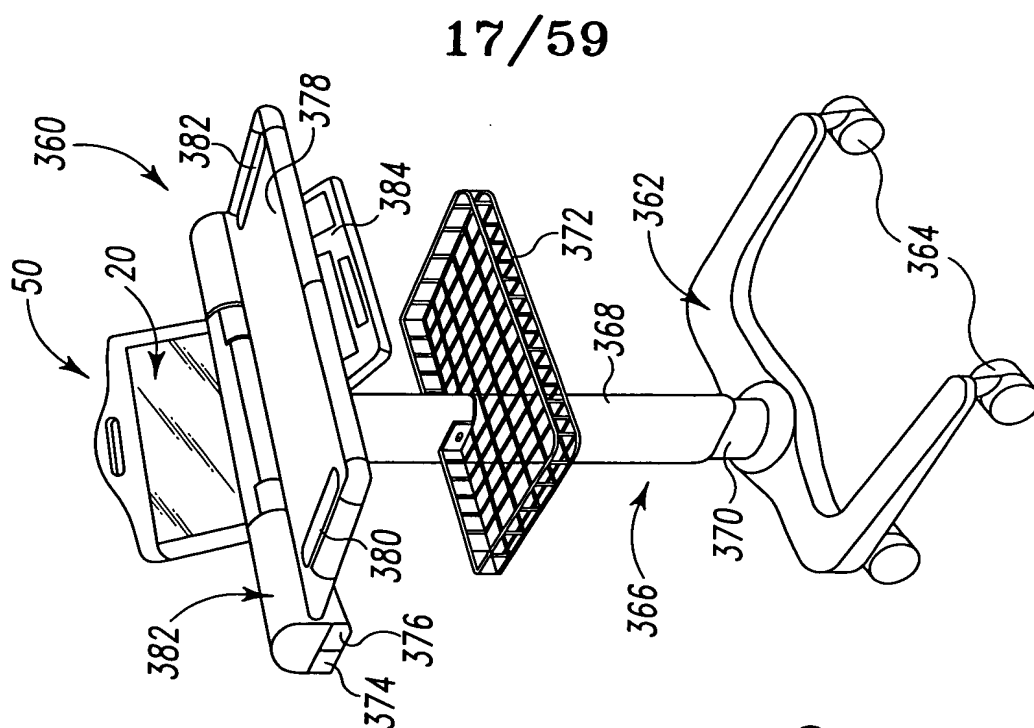


Fig. 31

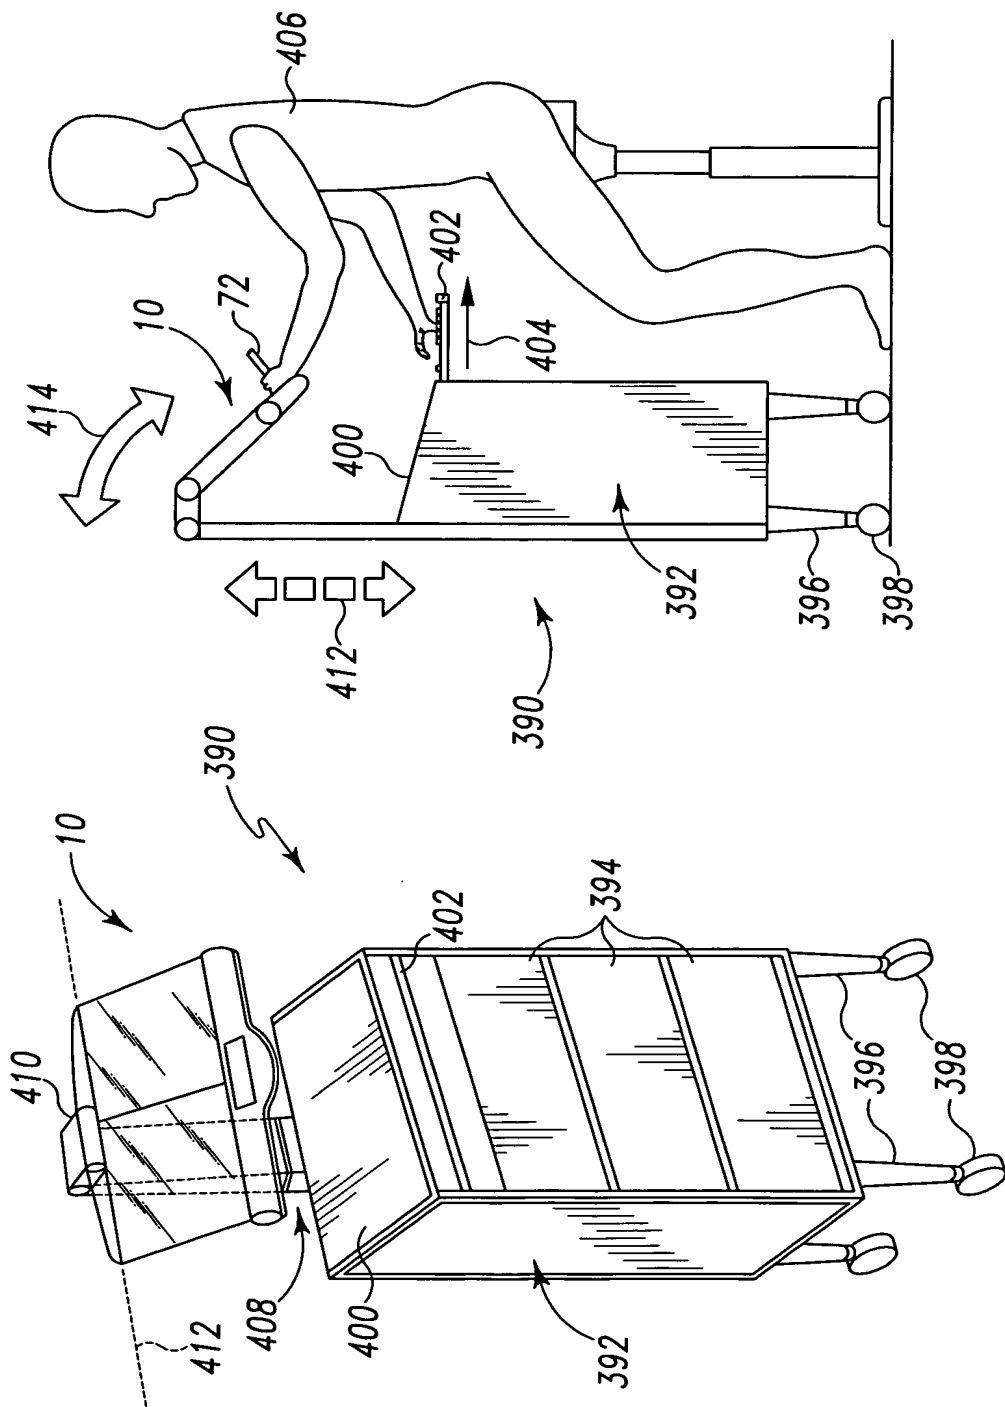


Fig. 33

Fig. 32

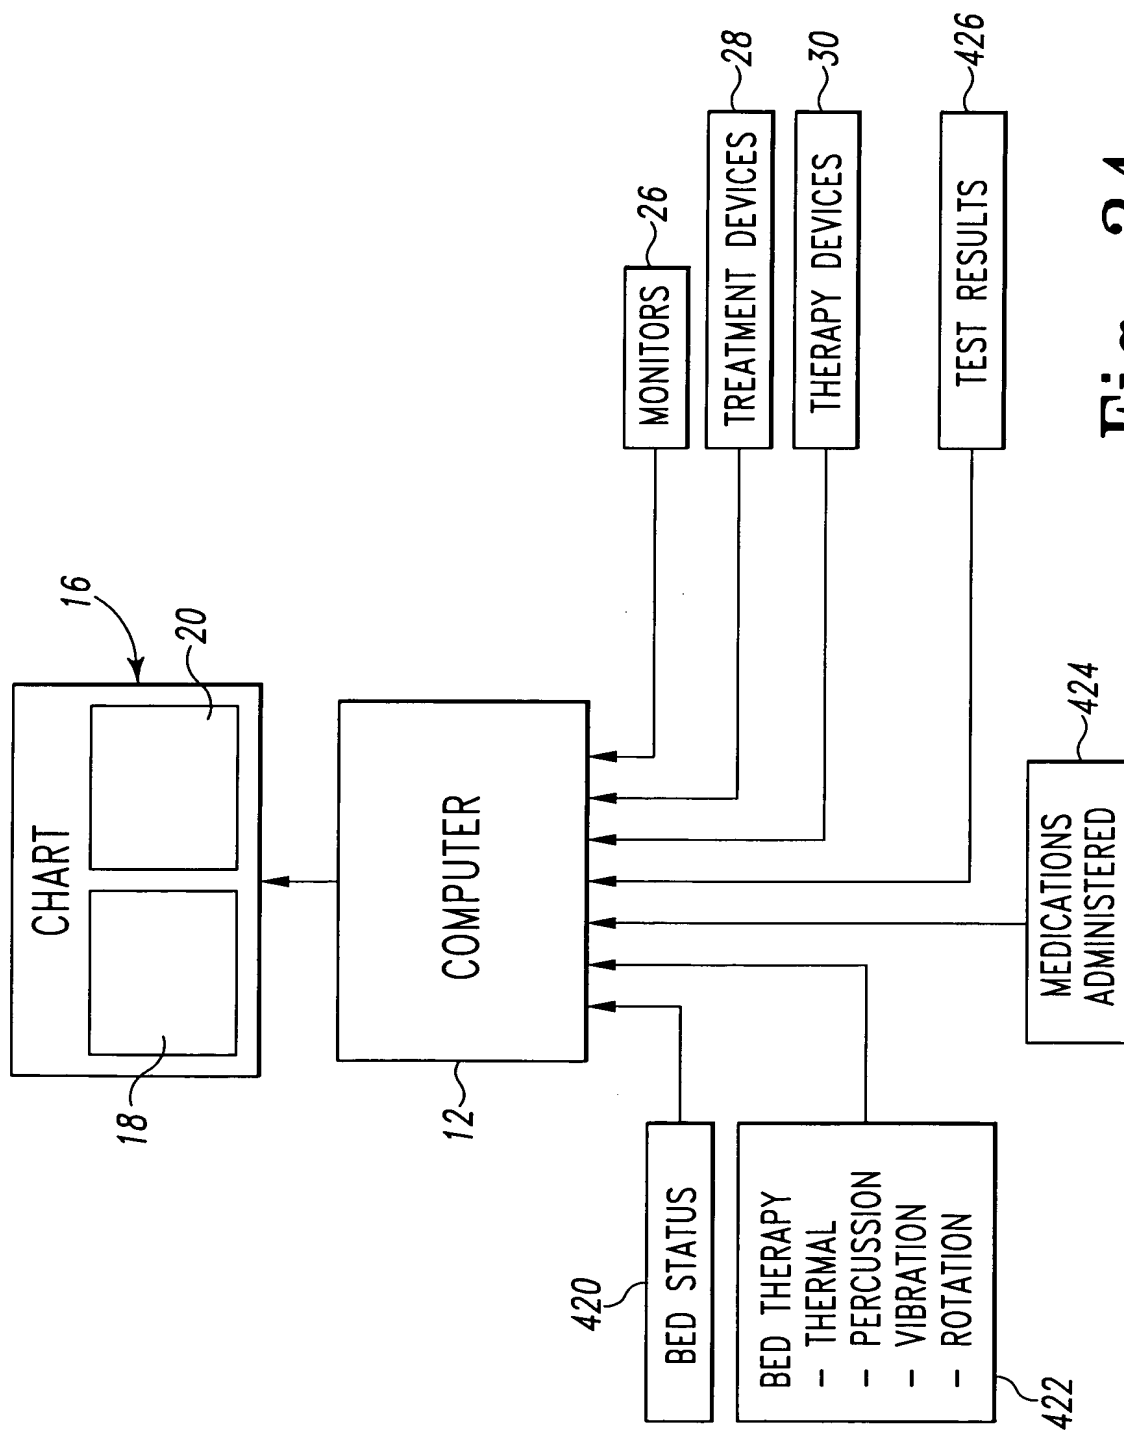


Fig. 34

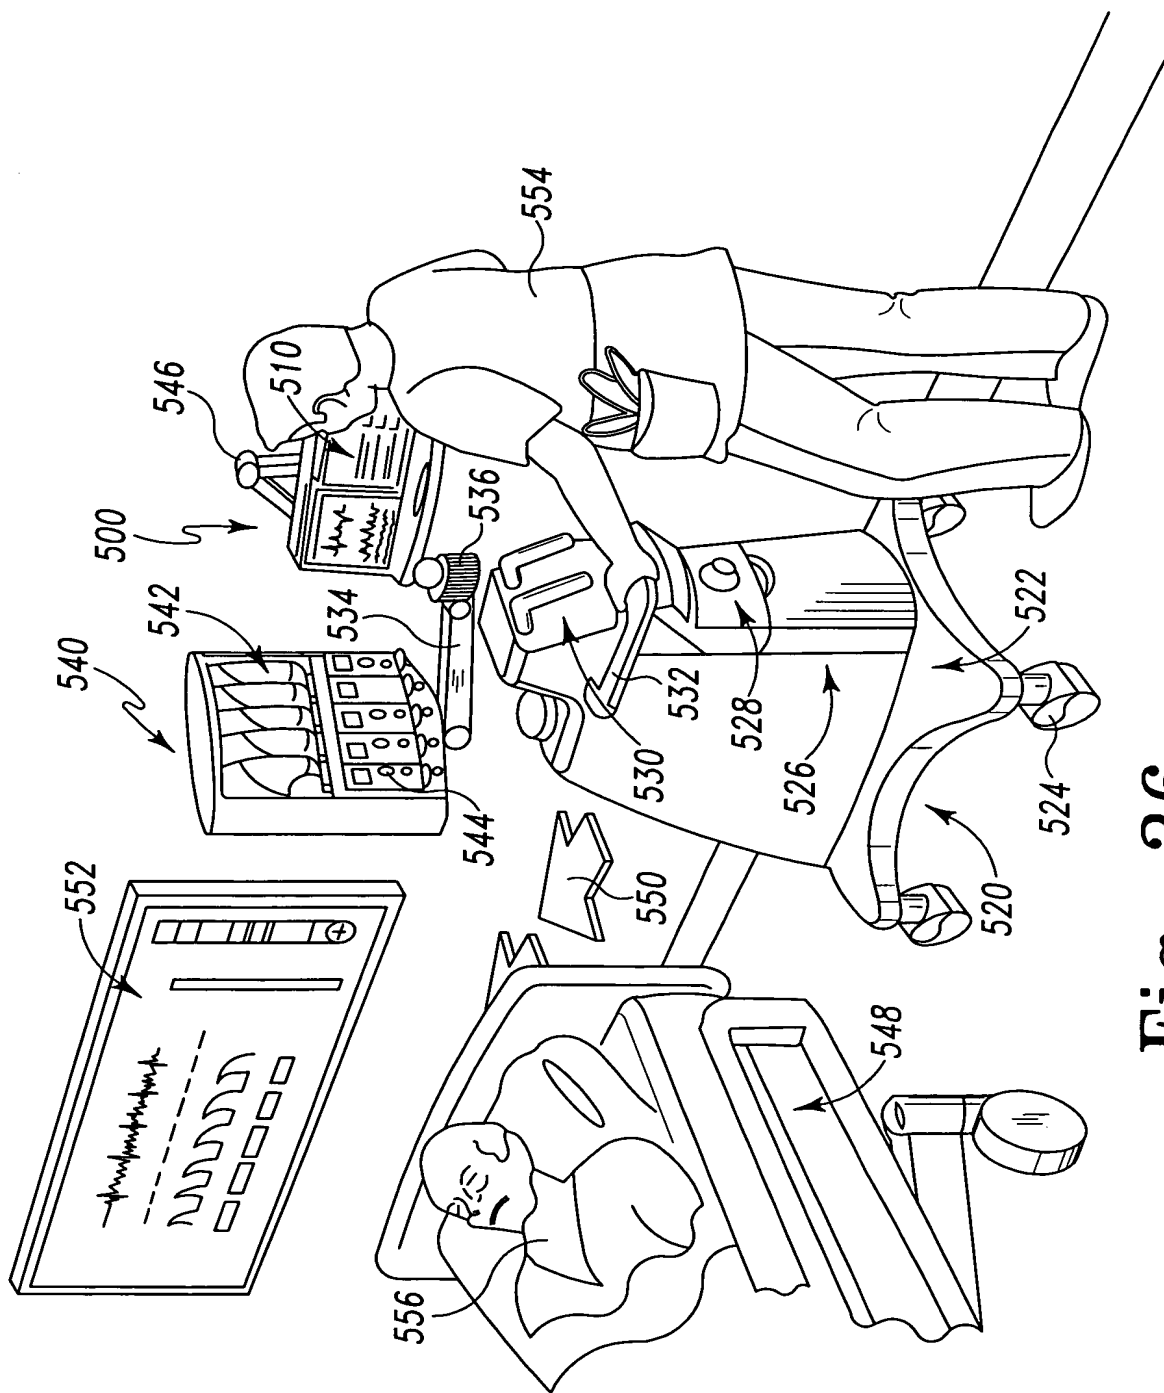


Fig. 36

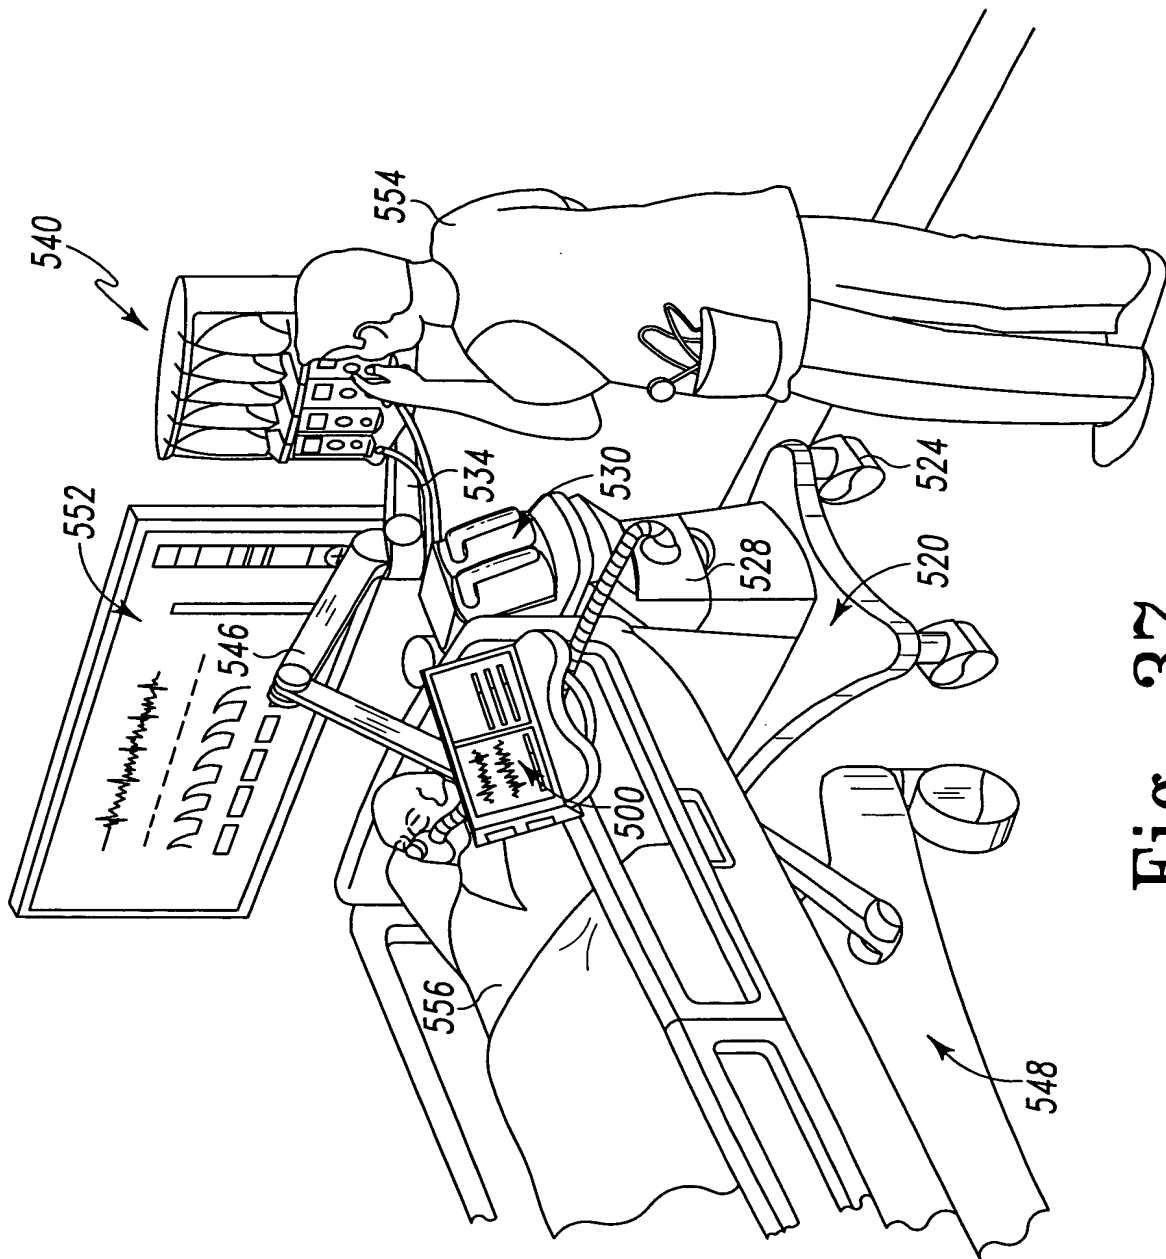


Fig. 37

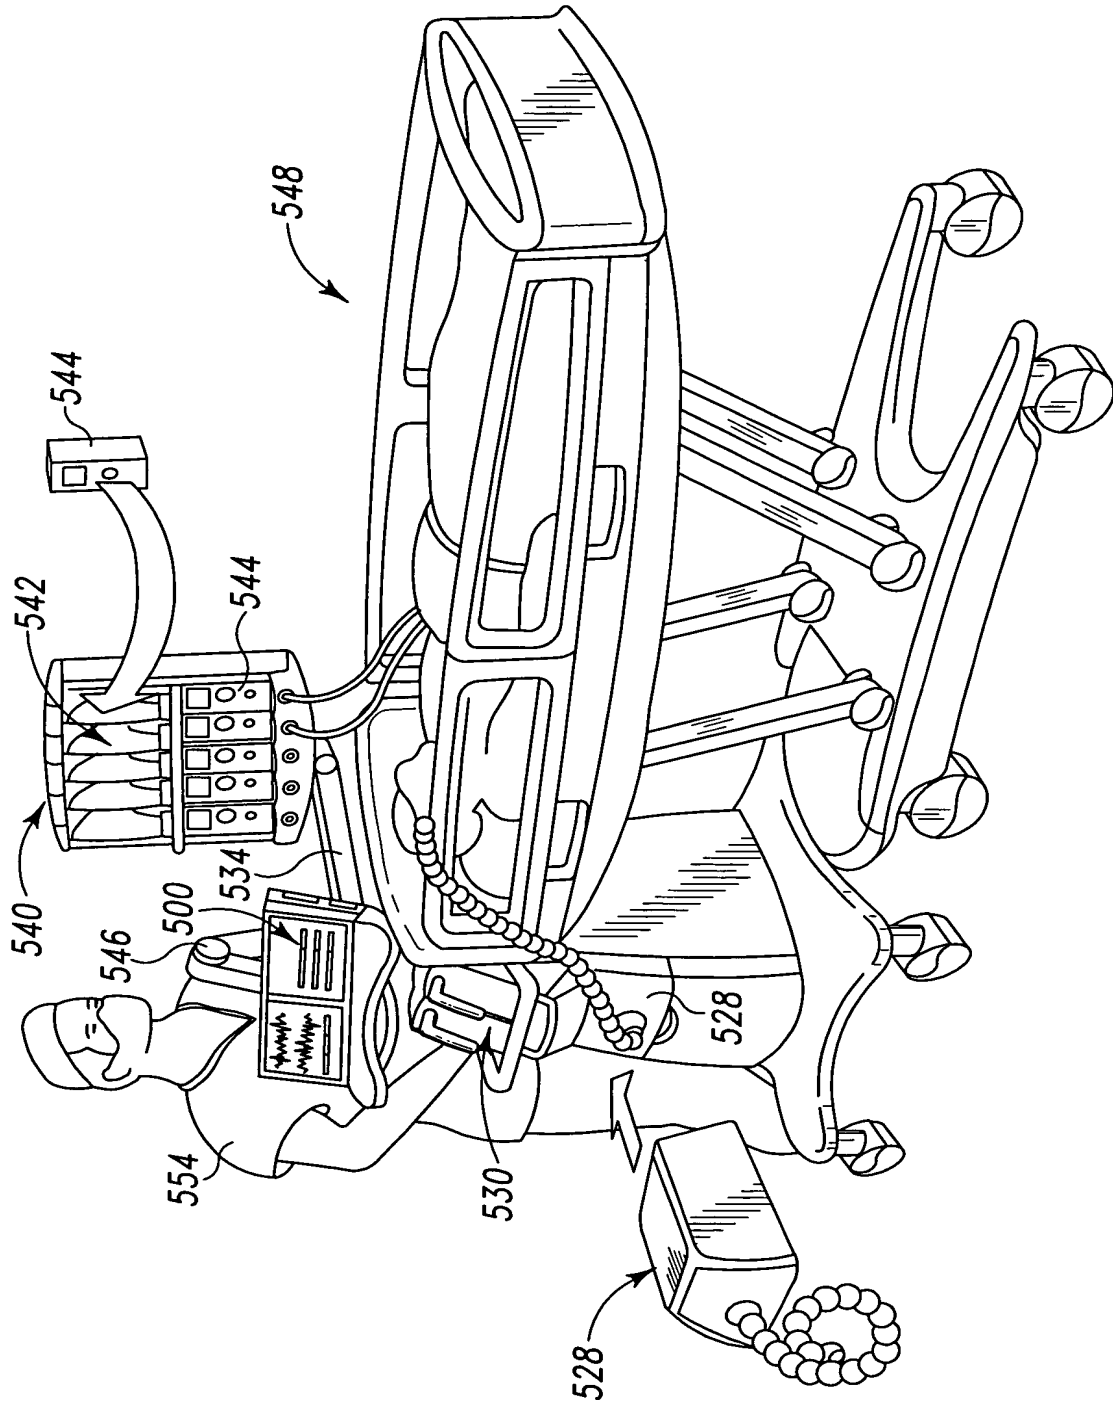


Fig. 38

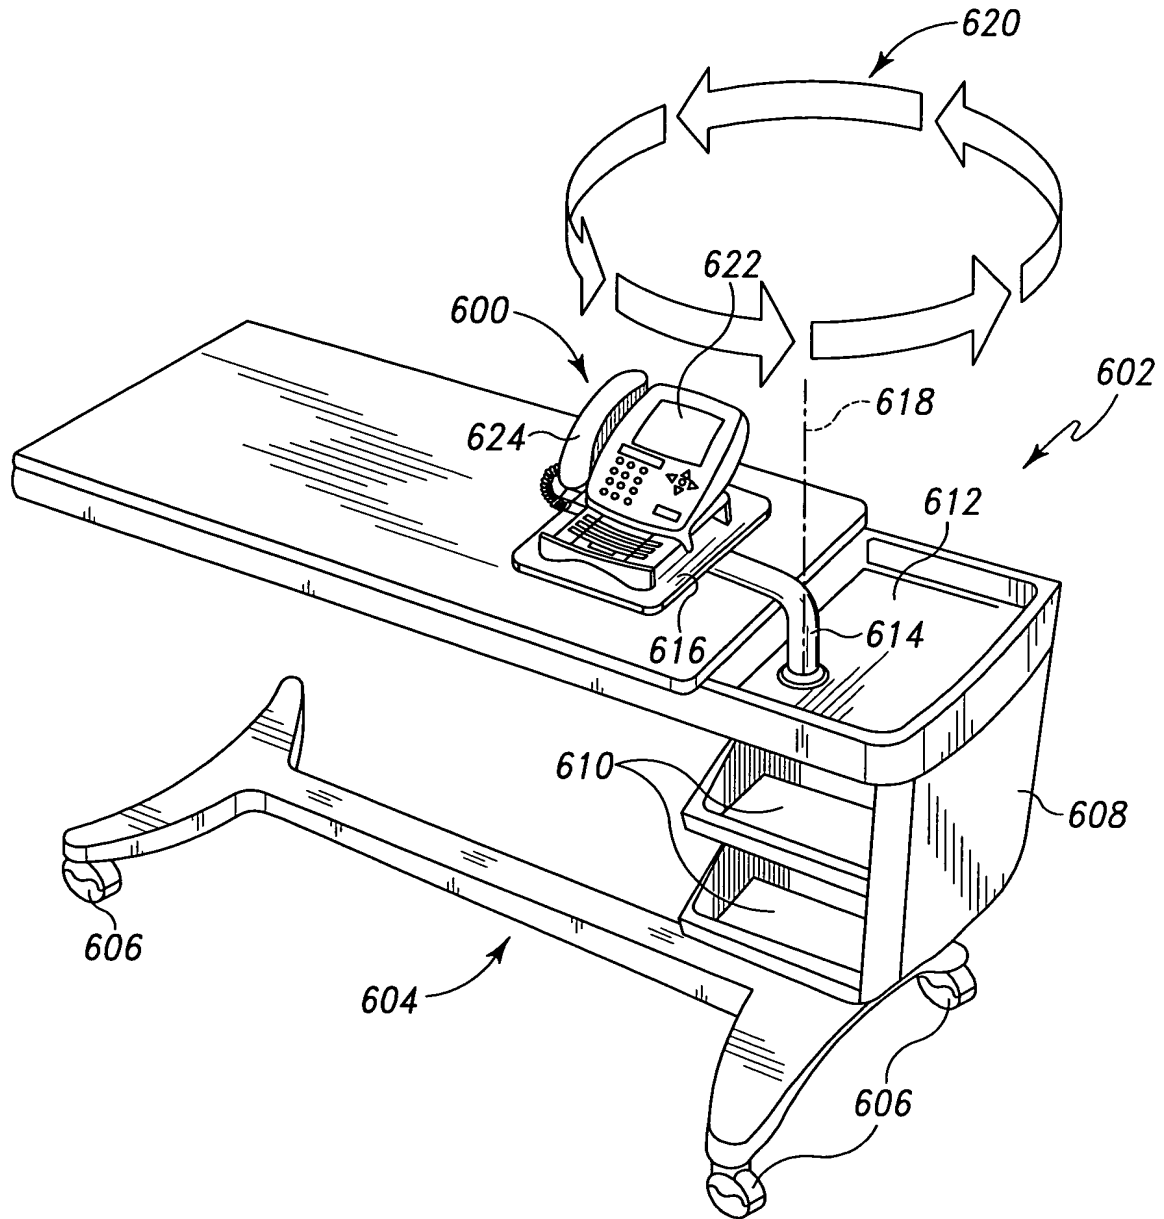


Fig. 39

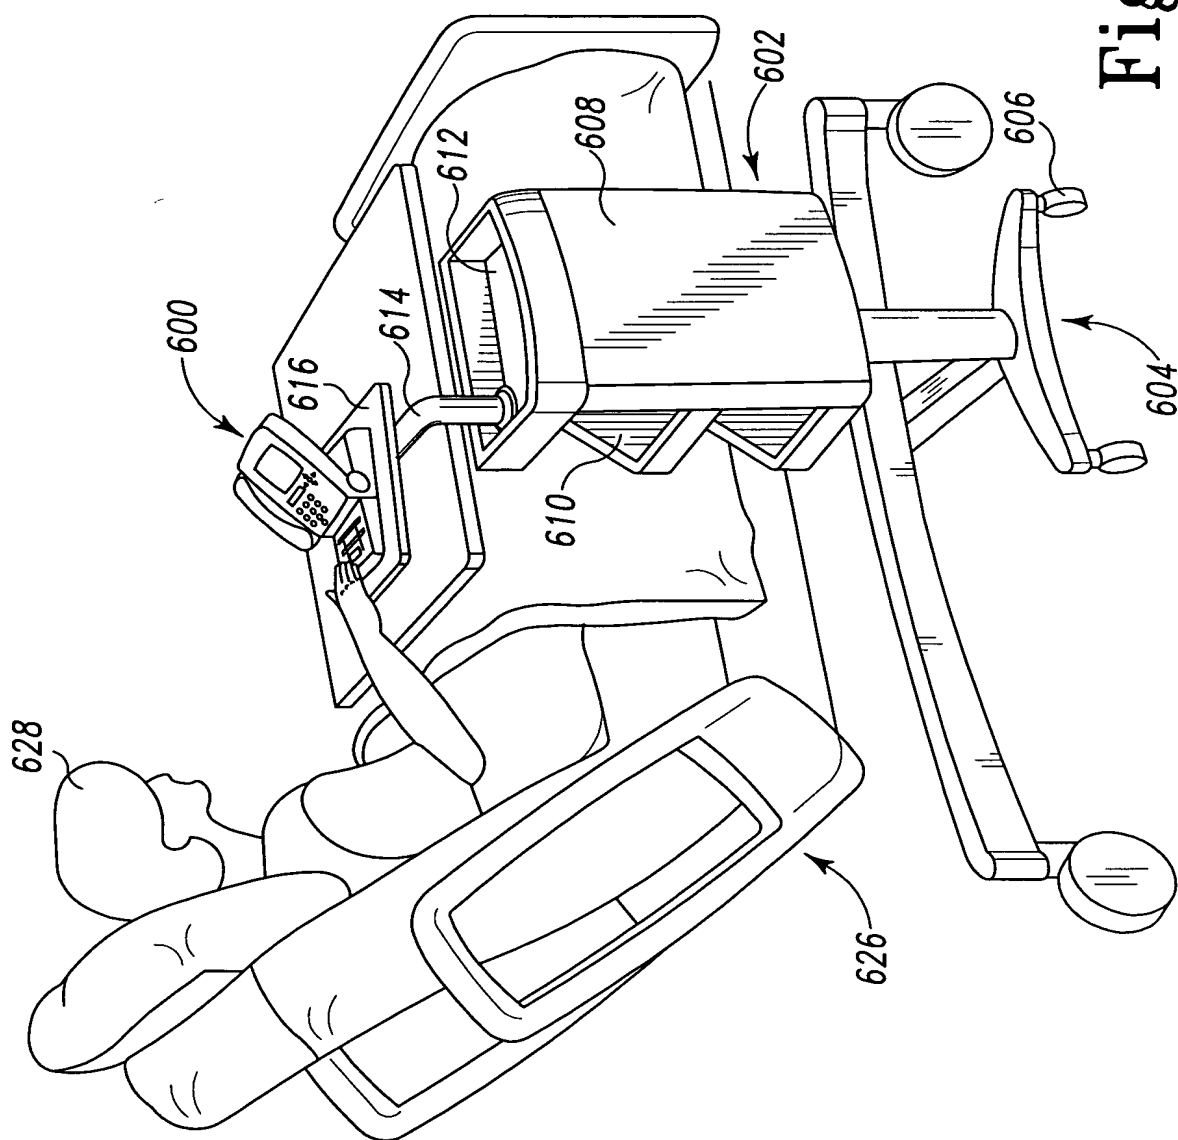


Fig. 40

FOSTER 08564860

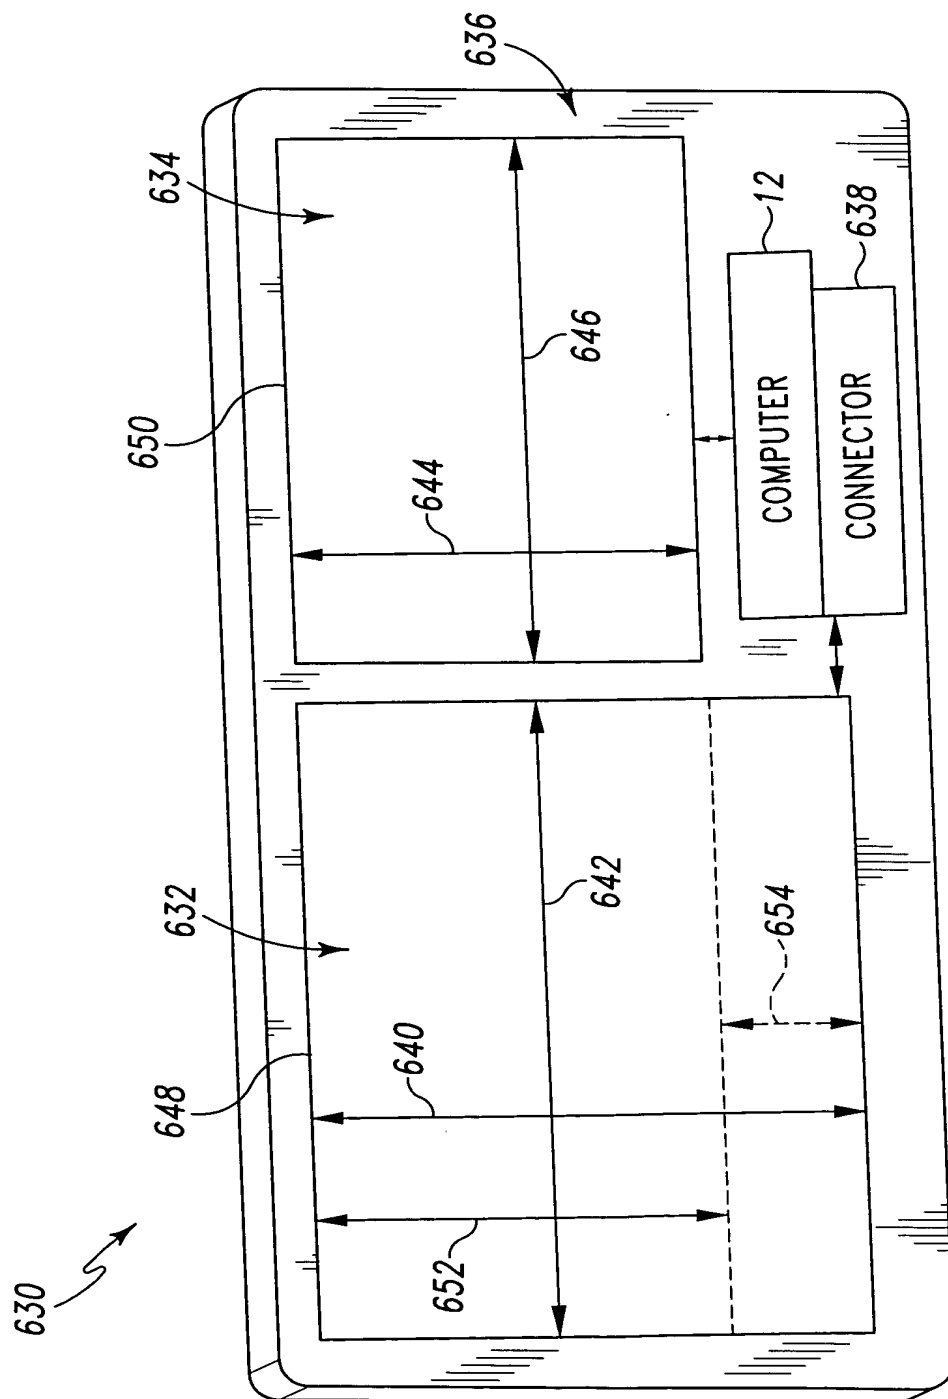


Fig. 41

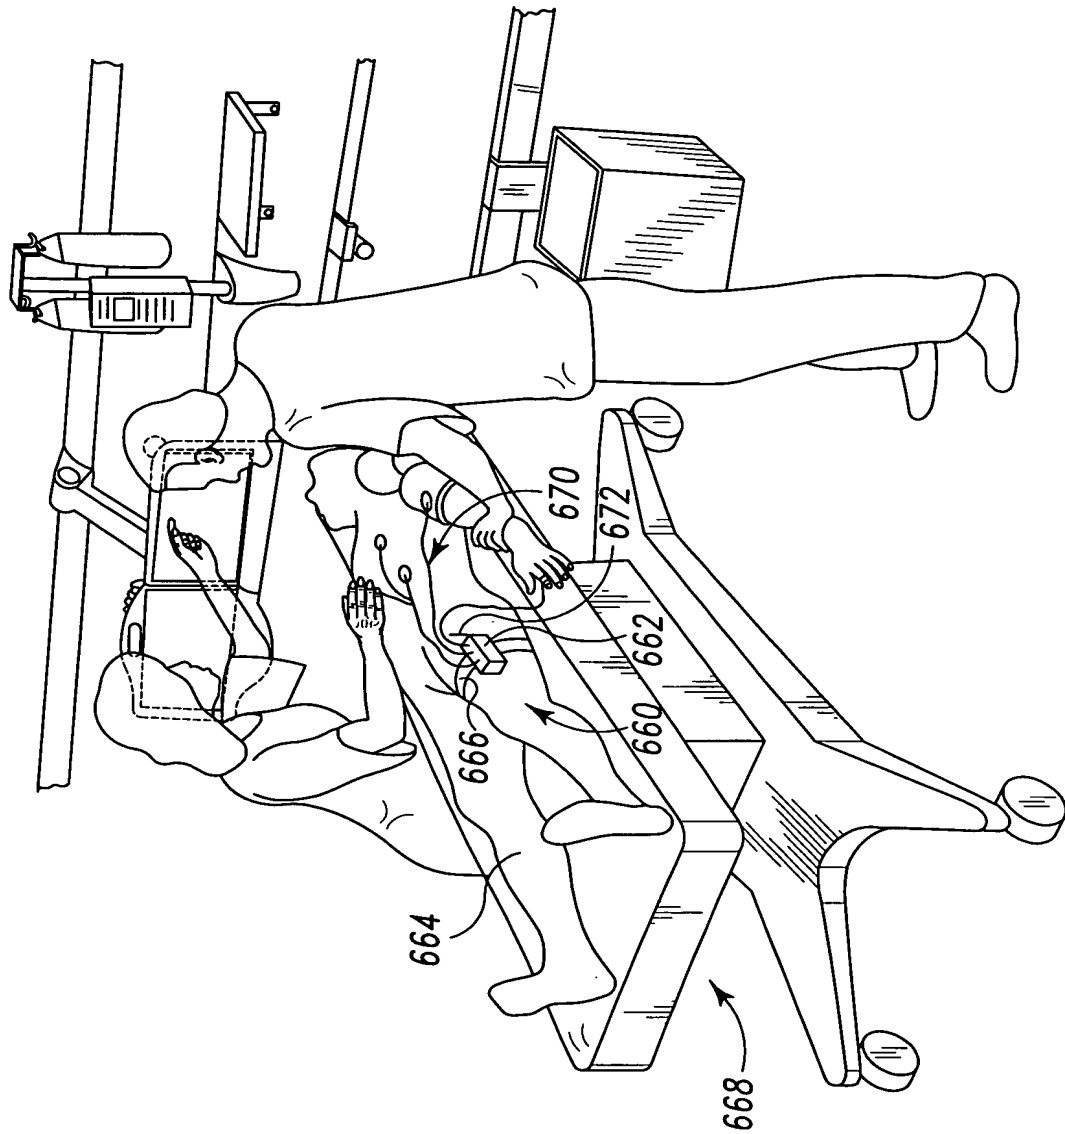


Fig. 42

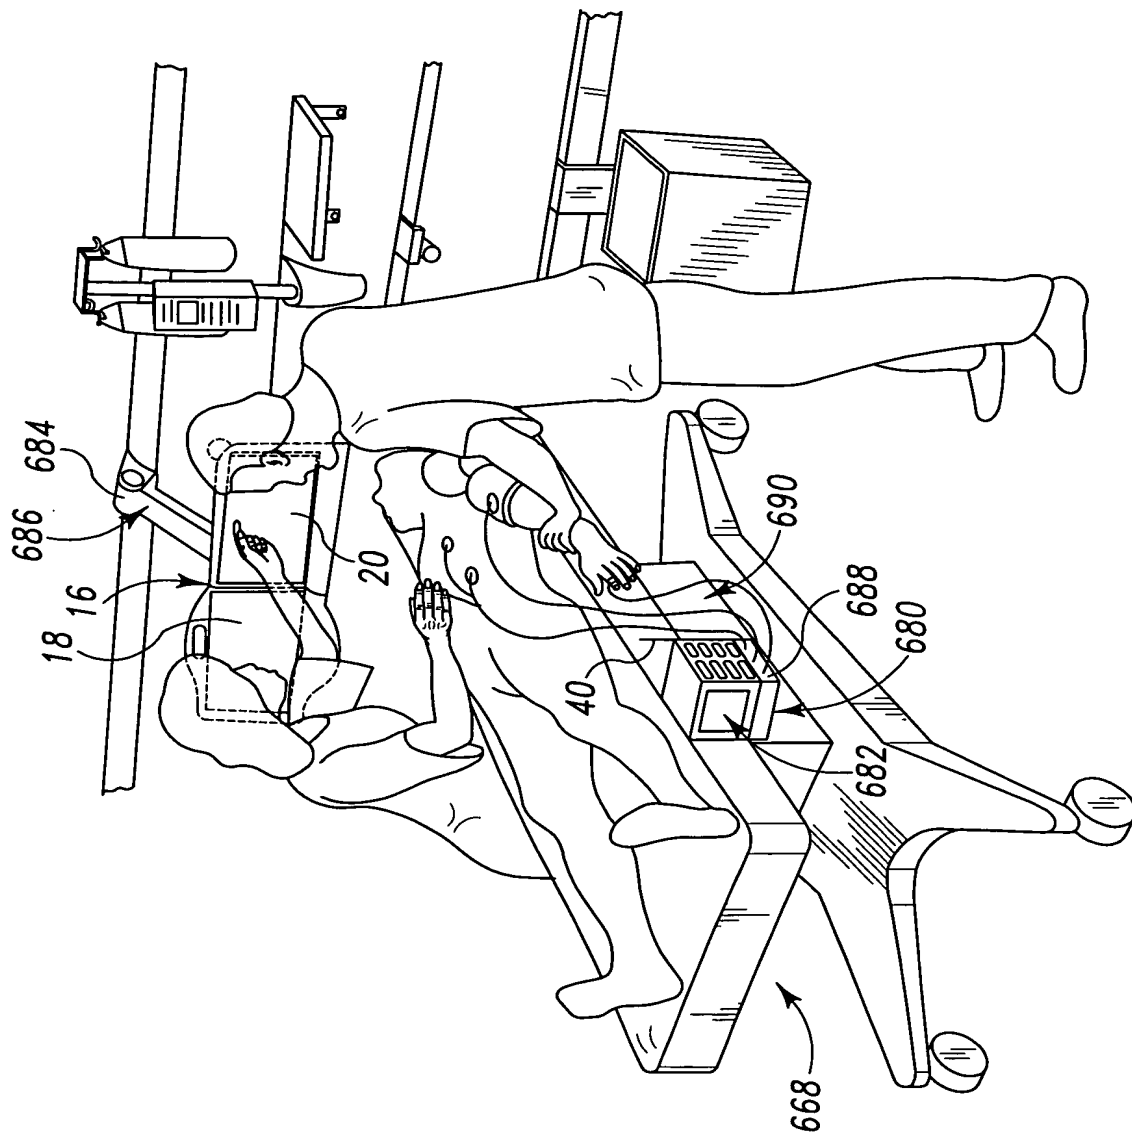


Fig. 43

29/59

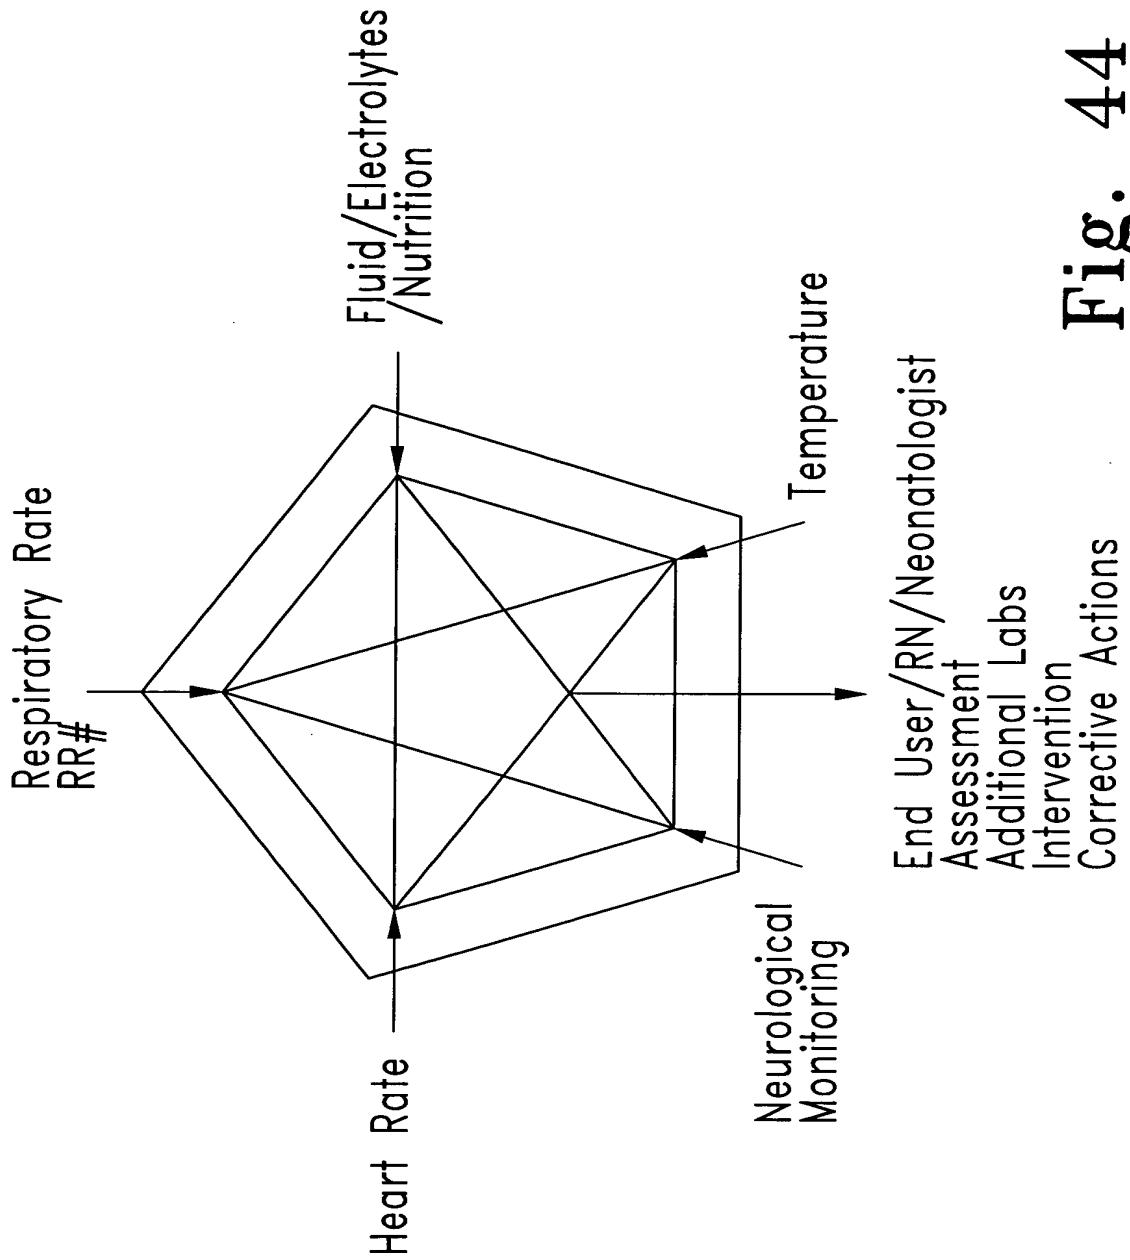


Fig. 44

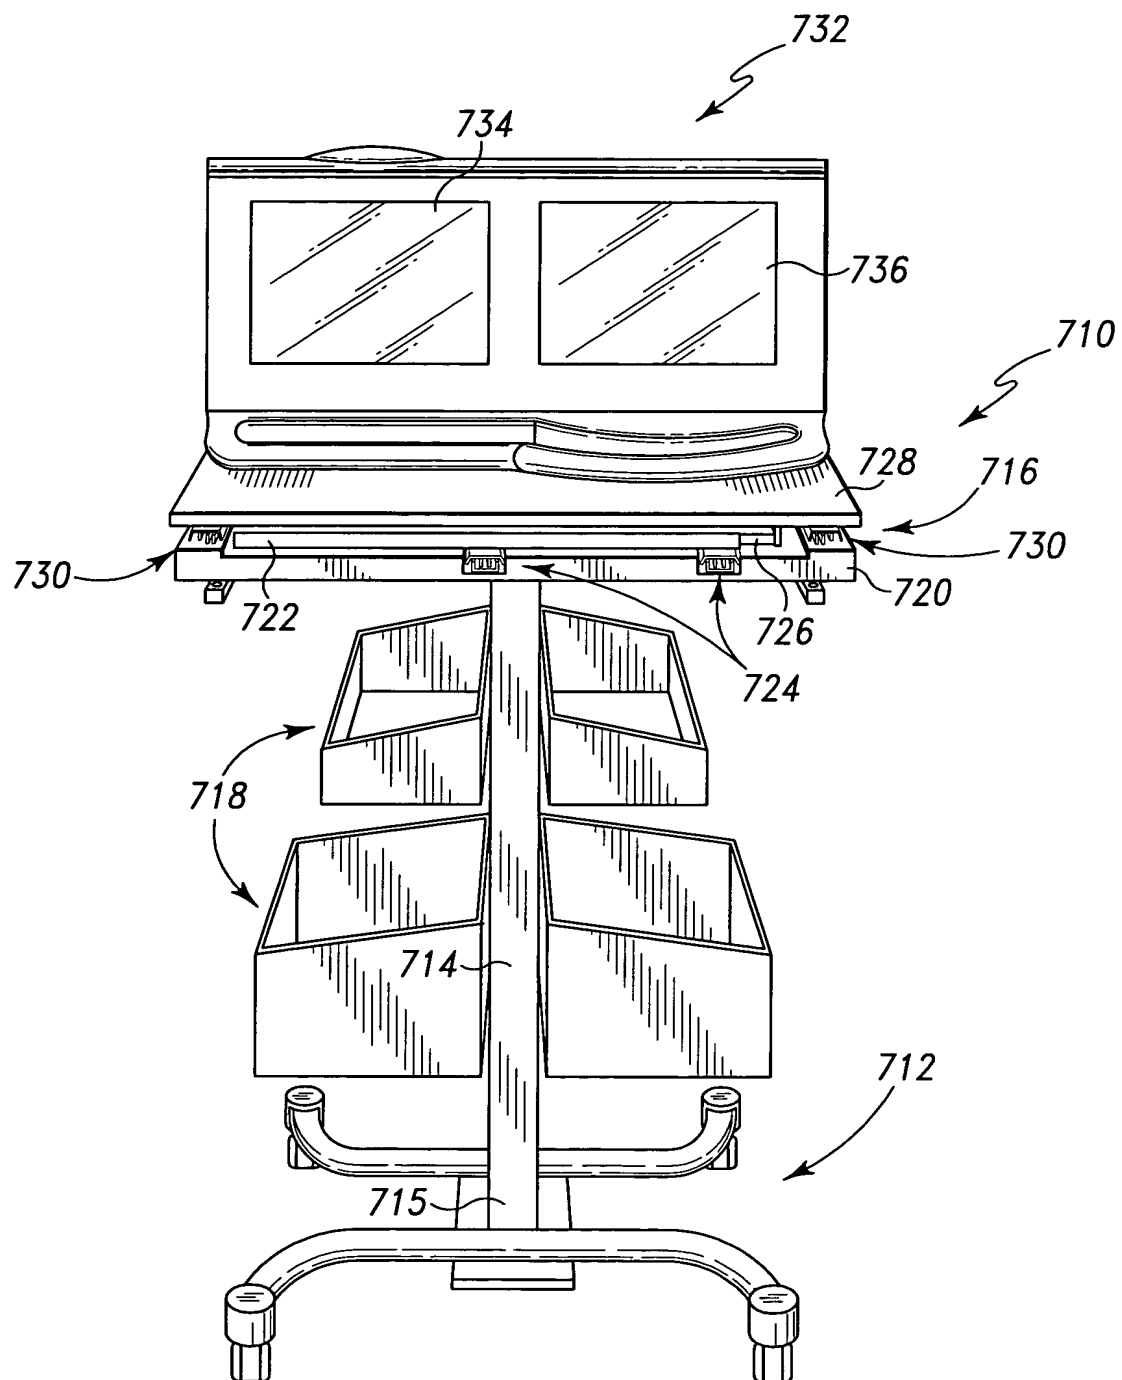


Fig. 45

31/59

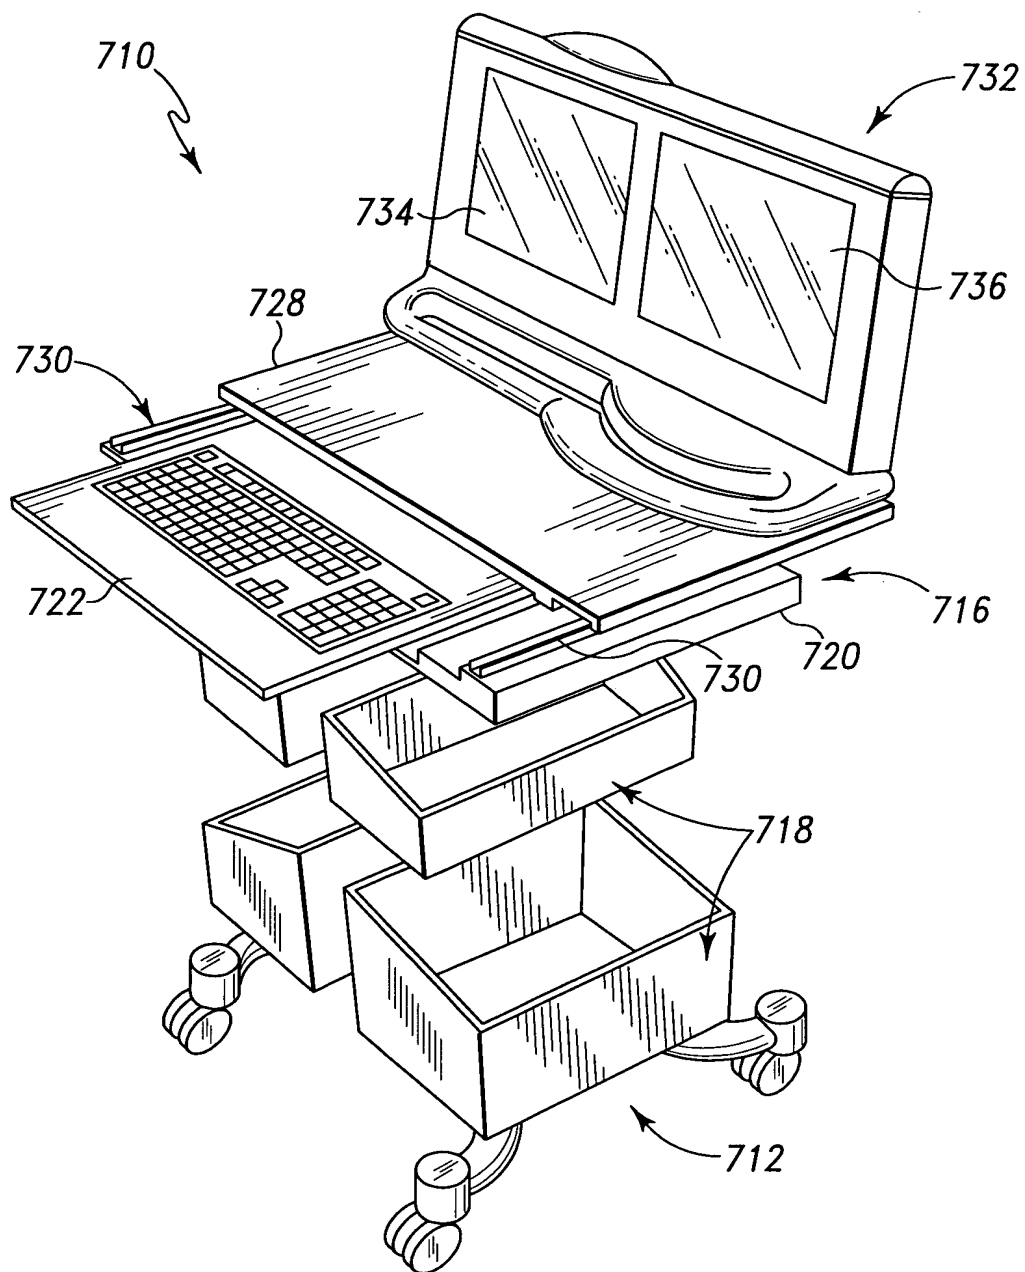


Fig. 46

09349580.121801


JOHN SMITH			6/24/00		11:05		
VITALS		TRENDS	P.INFO	SET-UP	HISTORY	EQUIP.	CPR
TIME			10:00	11:00	12:00	1:00	2:00
CORE TEMP			39.2	39.2	39.2	39.2	39.2
HEART RATE			107	108	107	107	107
HEART RHYTHM			S TACH	S TACH	S TACH	S TACH	S TACH
ART SYSTOLIC			150	160	150	150	150
ART DIASTOLIC			90	94	90	90	90
ART MEAN			110	116	110	110	110
PA SYSTOLIC			43	54	43	43	43
PA DIASTOLIC			22	25	22	22	22
PA MEAN			30	30	30	30	30
PCMP			20	10	20	20	20
CVP			10	10	10	10	10
CO			4.70	4.70	4.70	4.70	4.70
CI			2.17	2.17	2.17	2.17	2.17
SVR			10.89	10.89	10.89	10.89	10.89
PVR			159	159	159	159	159
SV02			61	64	61	61	61
RESPIRATORY RATE			15	11	15	15	15
SPO2			100	99	100	100	100

Fig. 47A

JOHN SMITH

6/24/00

11:05

3:00	4:00	5:00	6:00
39.2	39.2	39.2	39.2
107	107	107	107
S TACH	S TACH	S TACH	S TACH
150	150	150	150
90	90	90	90
110	110	110	110
43	43	43	43
22	22	22	22
30	30	30	30
20	20	20	20
10	10	10	10
4.70	4.70	4.70	4.70
2.17	2.17	2.17	2.17
10.89	10.89	10.89	10.89
159	159	159	159
61	61	61	61
15	15	15	15
100	100	100	100

0

9

9

A

Q

Z

ENTER

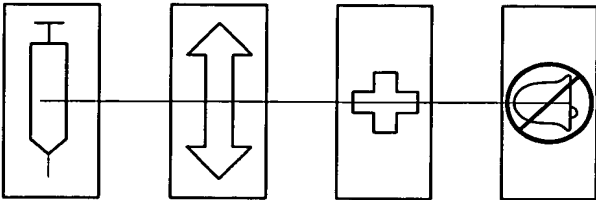
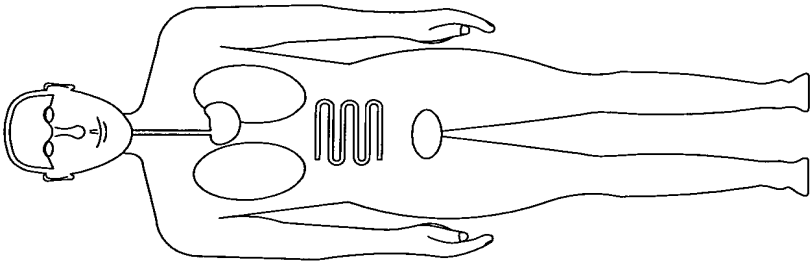


Fig. 47B

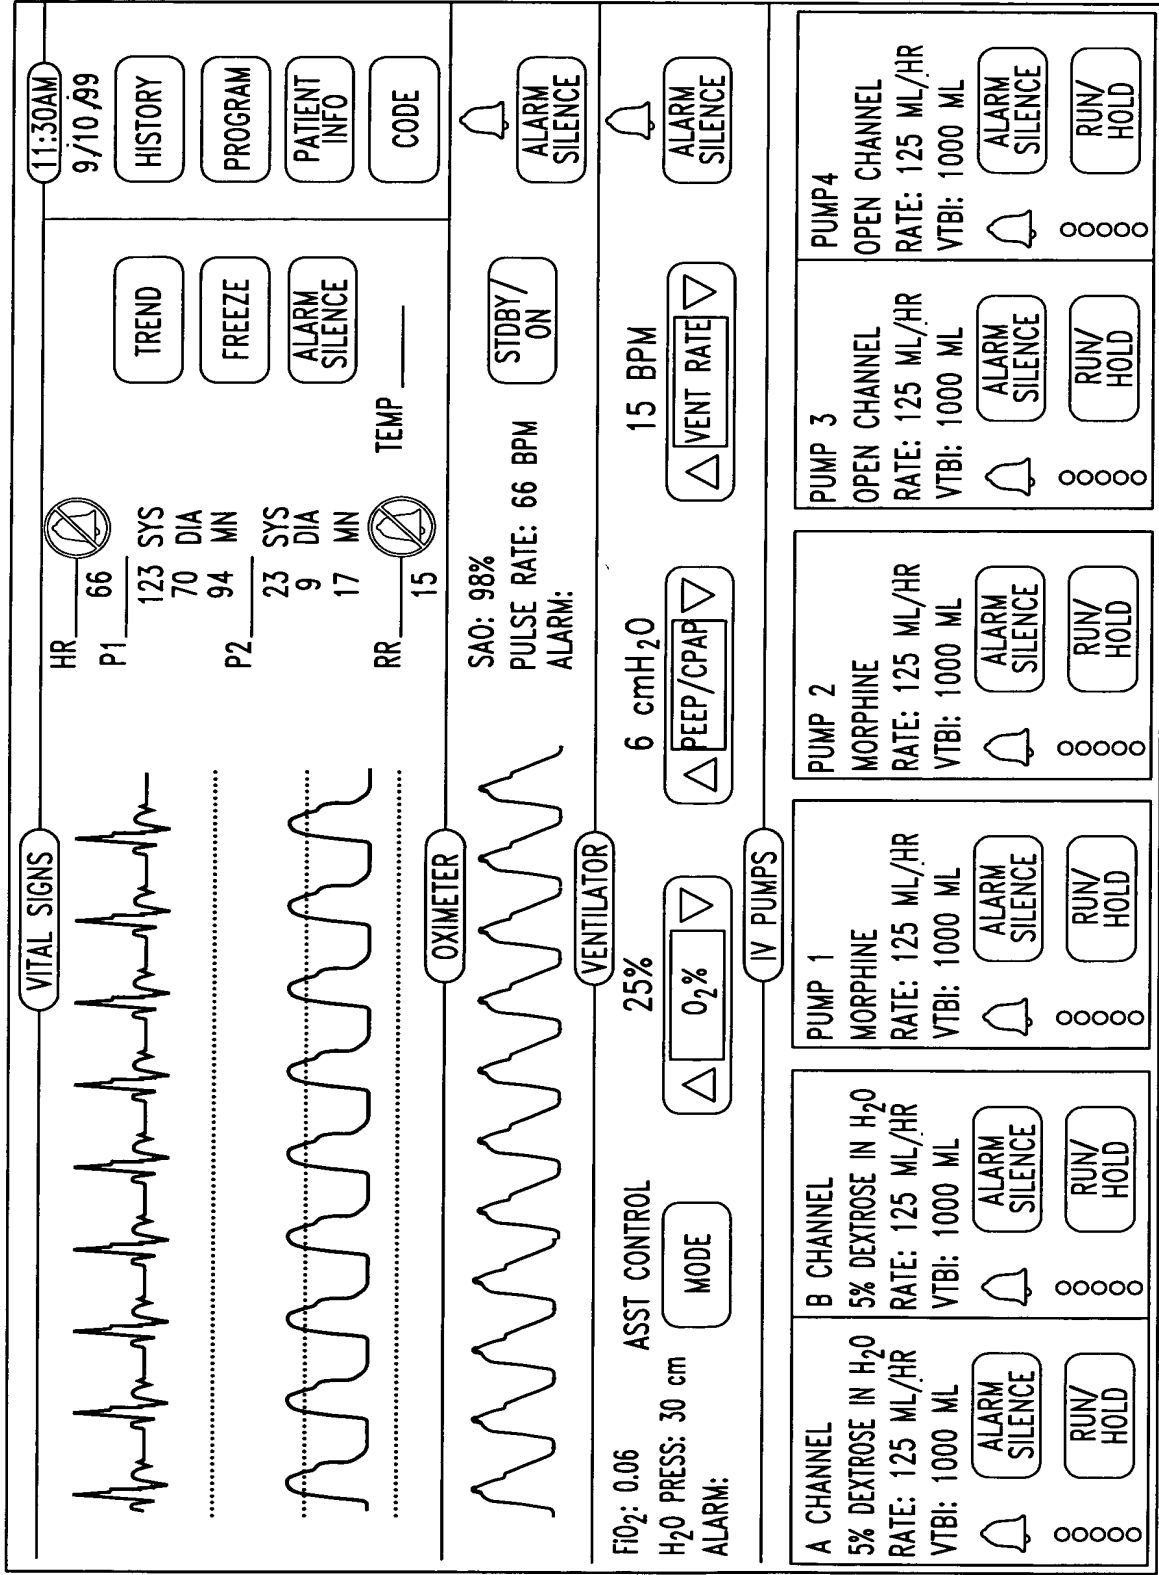


Fig. 48

35/59




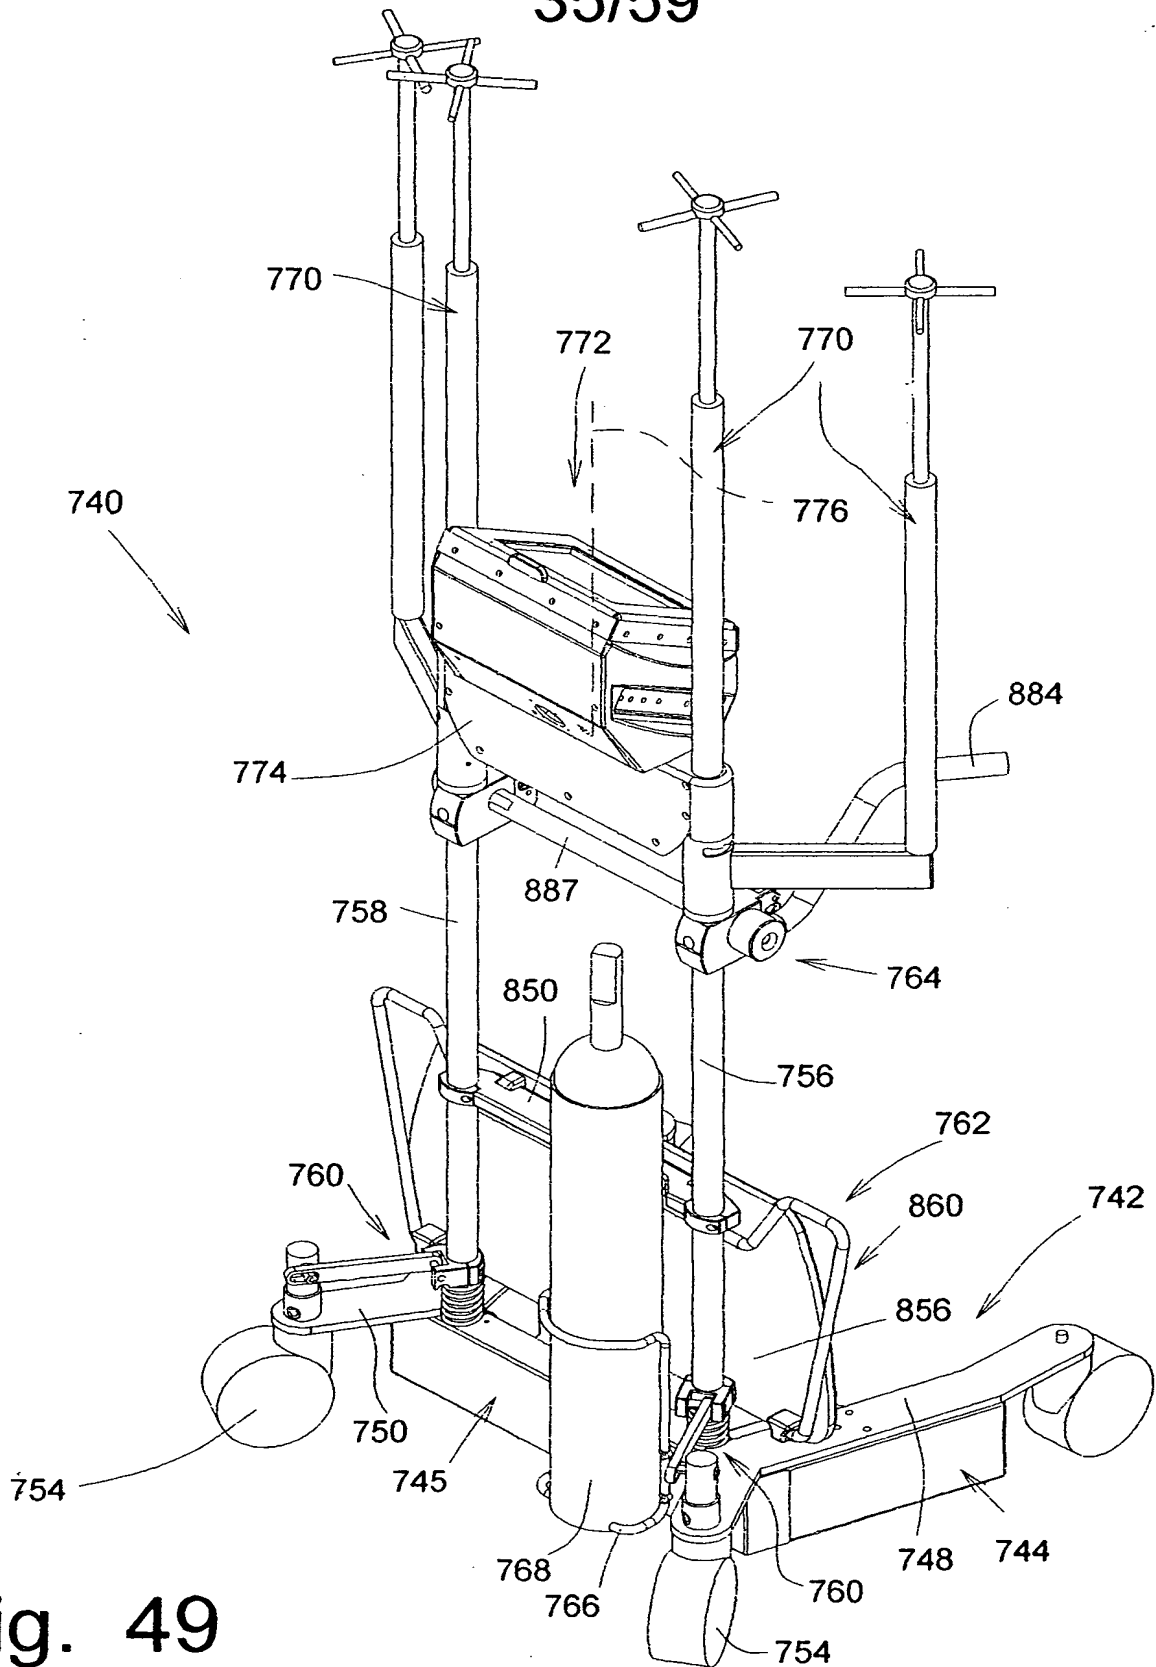


Fig. 49

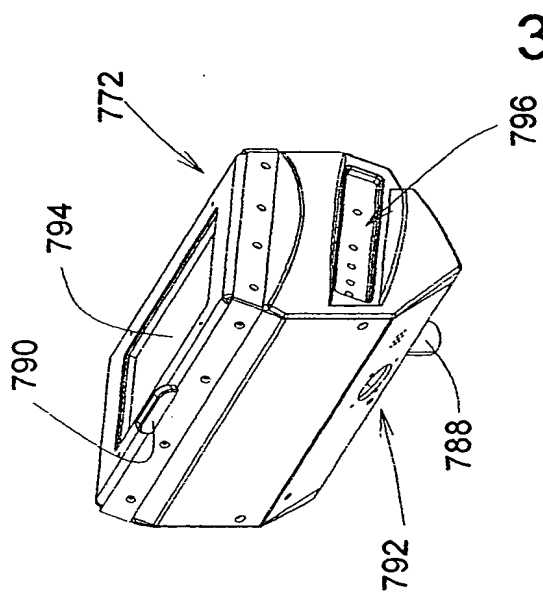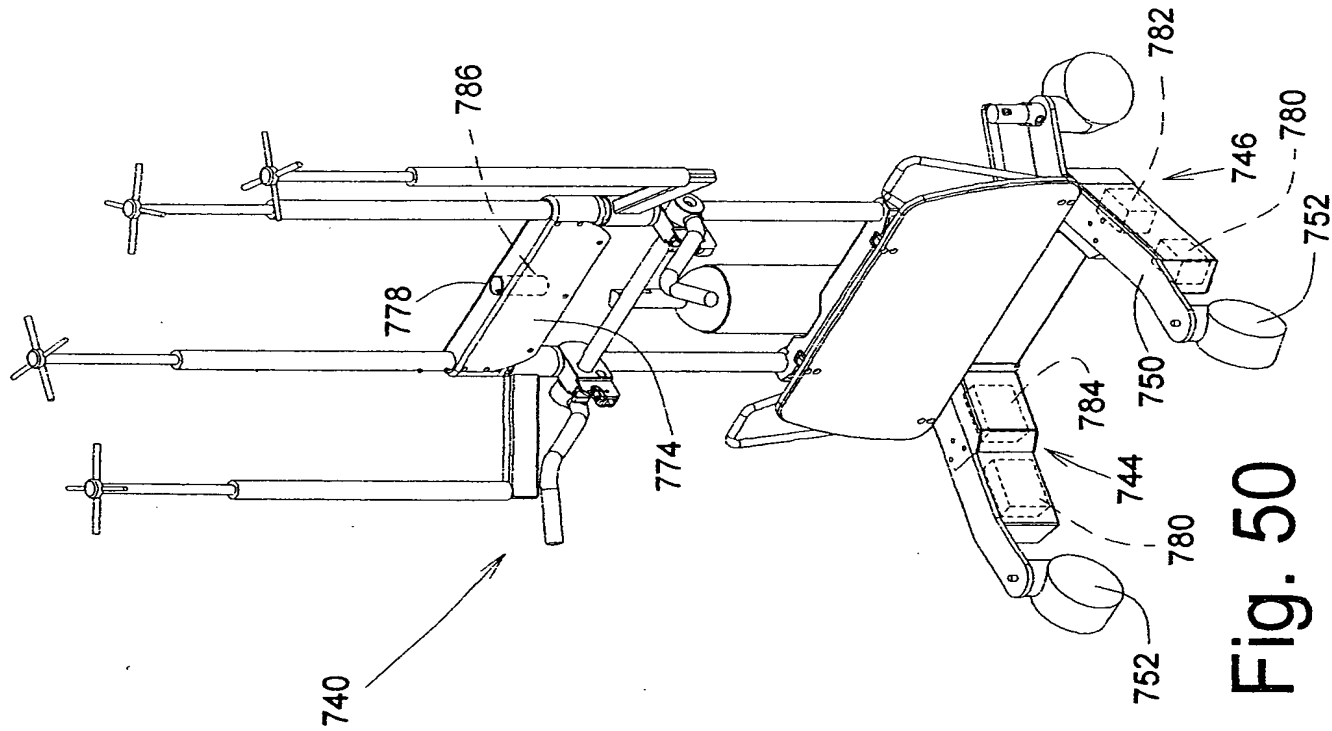

36/59

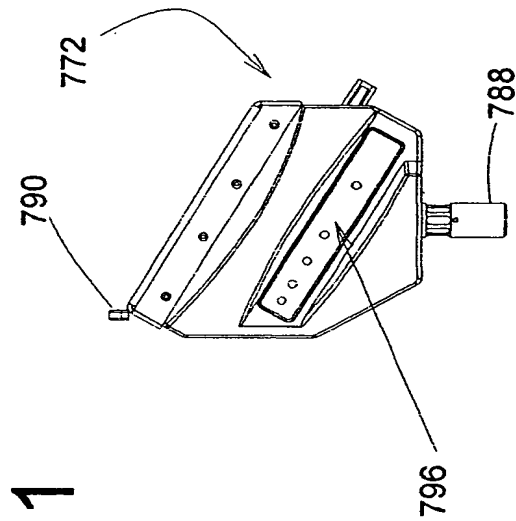

37/59

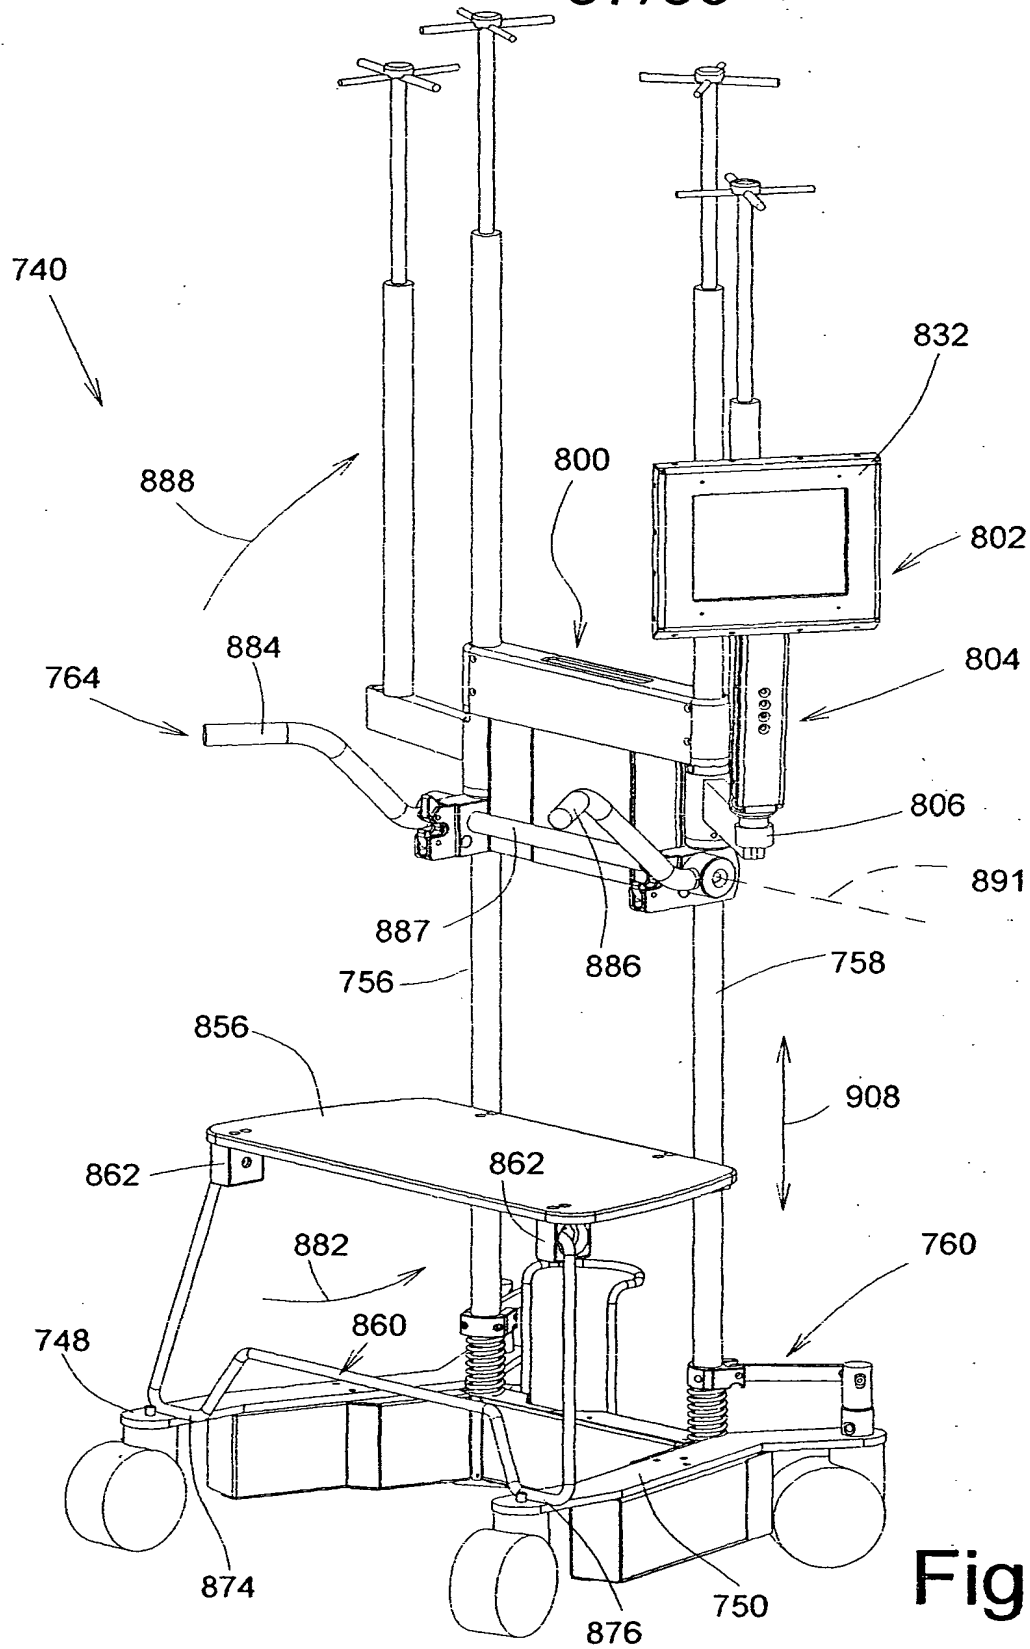


Fig. 53

38/59

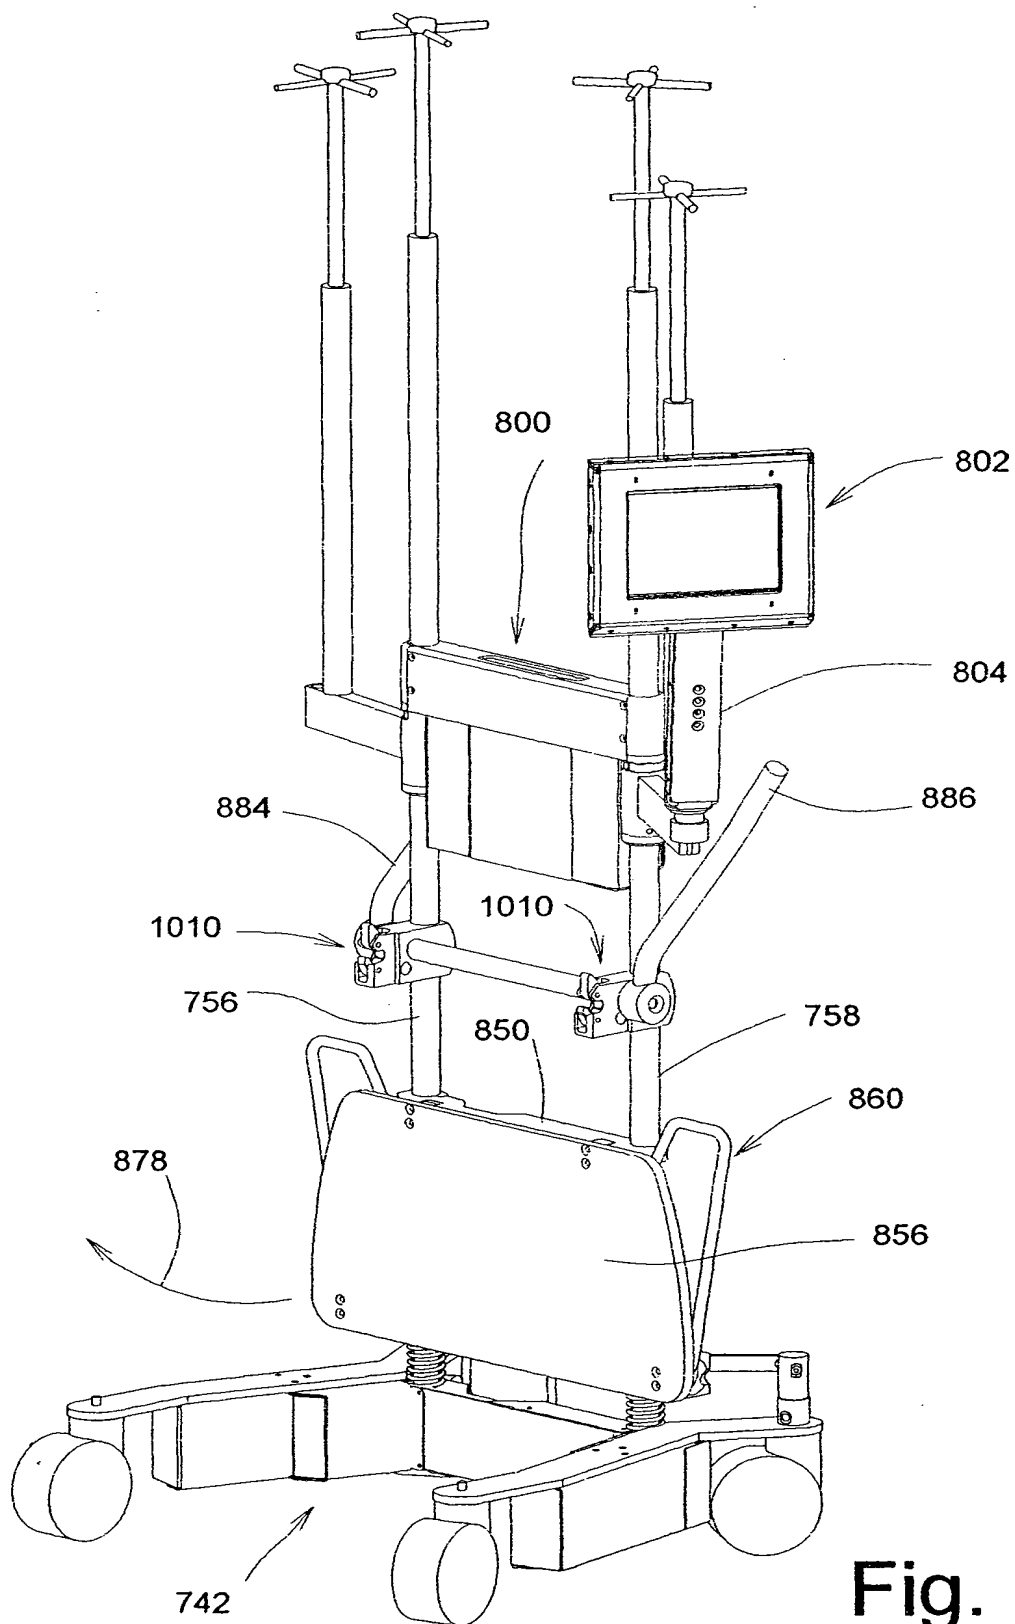


Fig. 54

09849580-121801

39/59

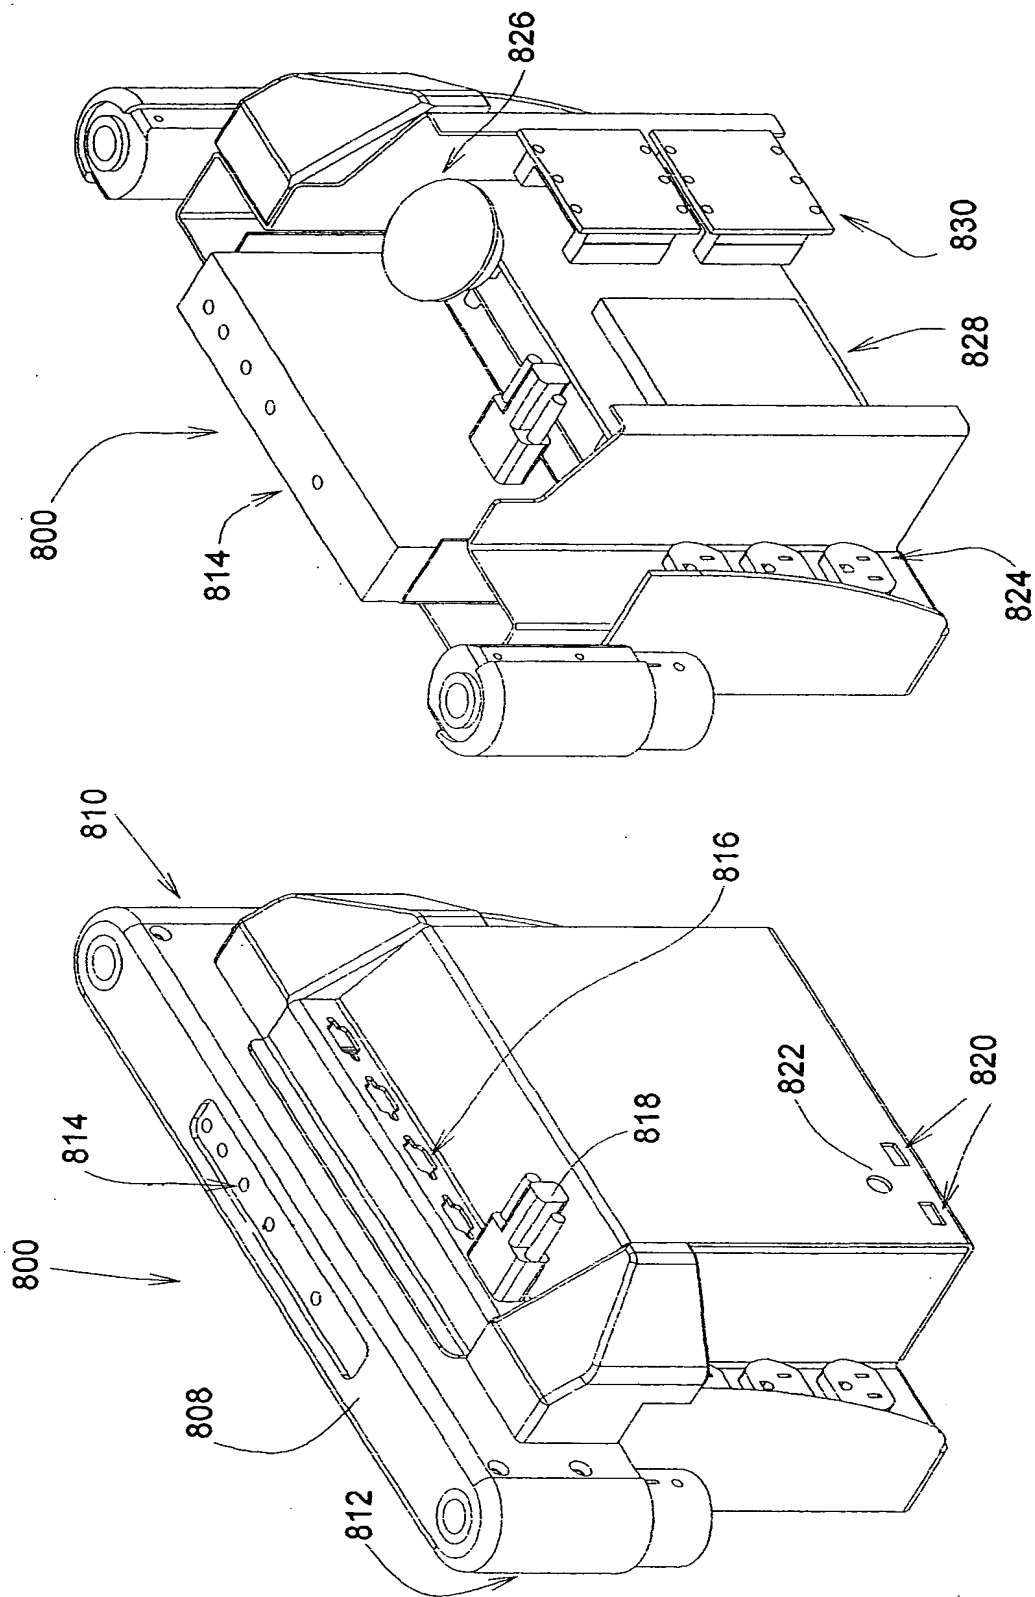


Fig. 56

Fig. 55

40/59

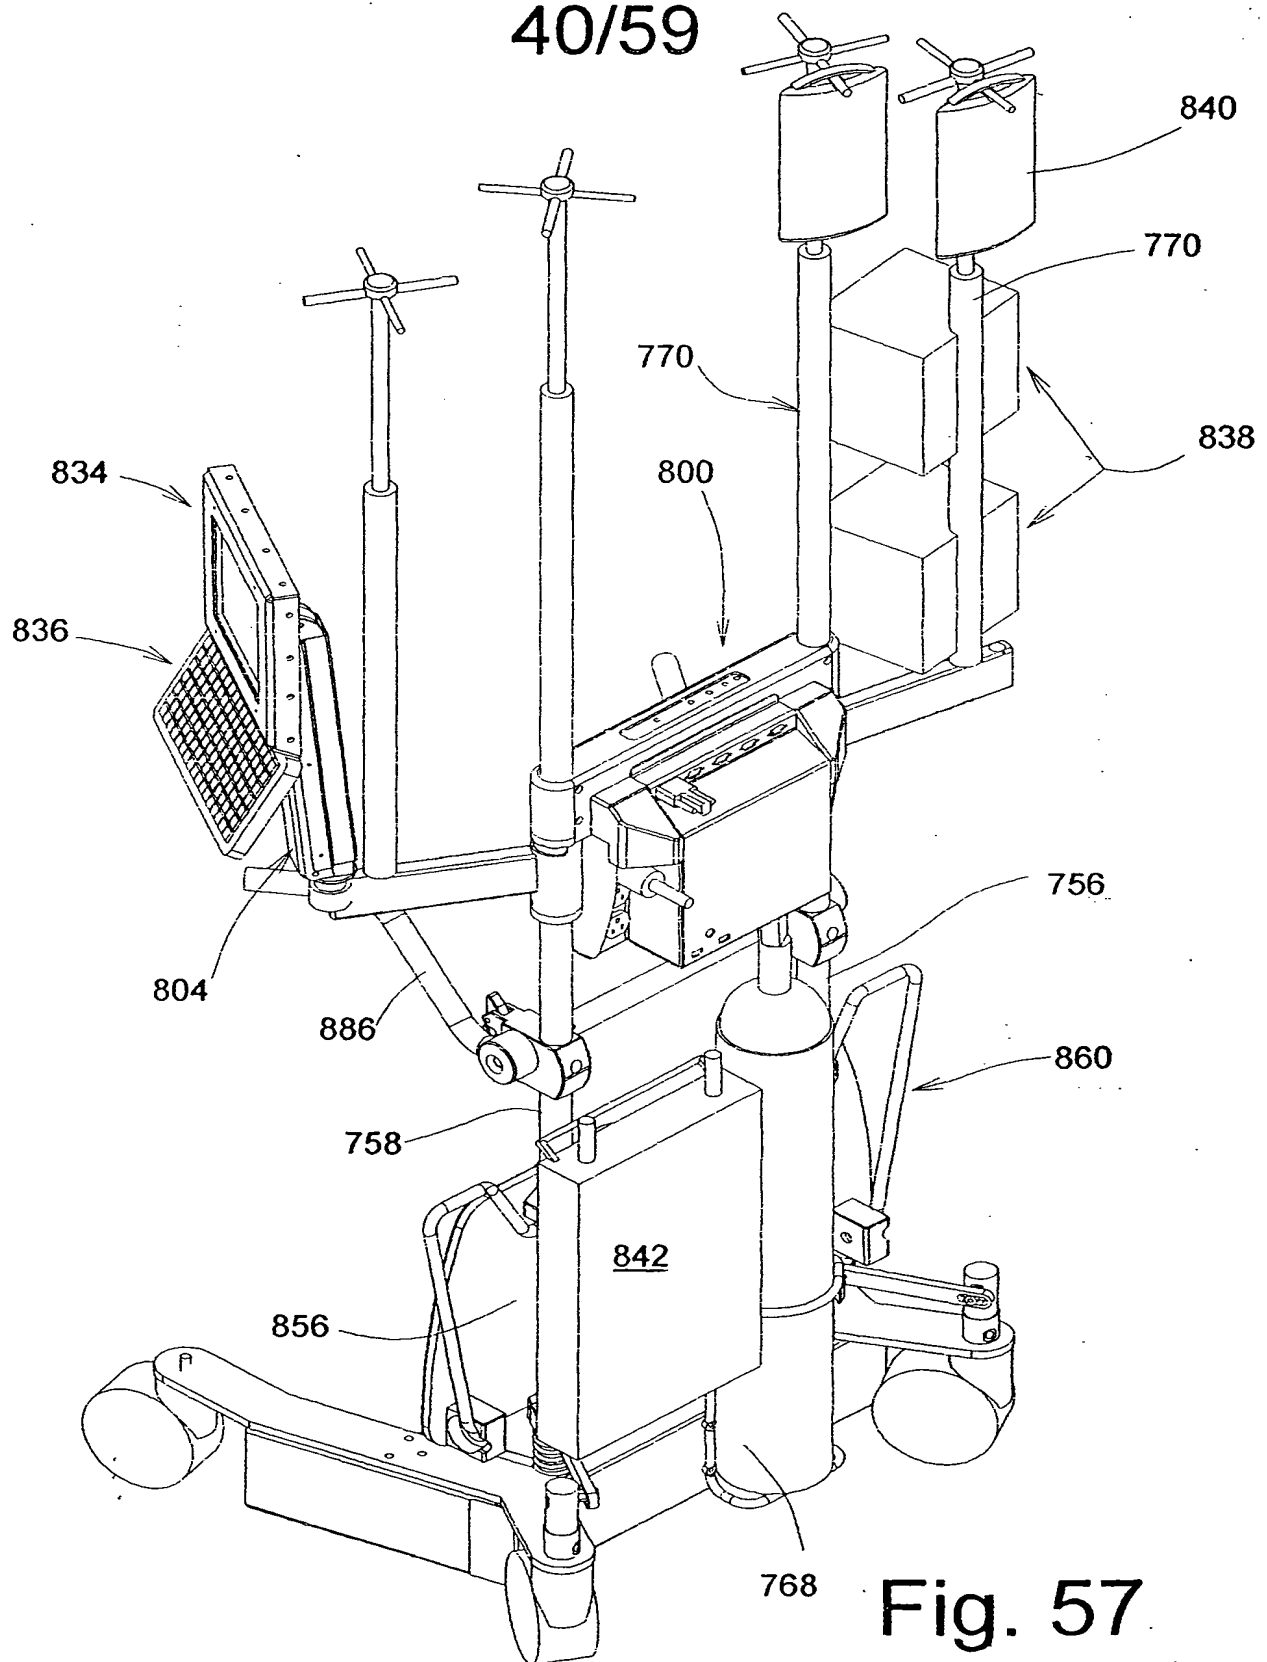


Fig. 57

09849580-121801

41/59


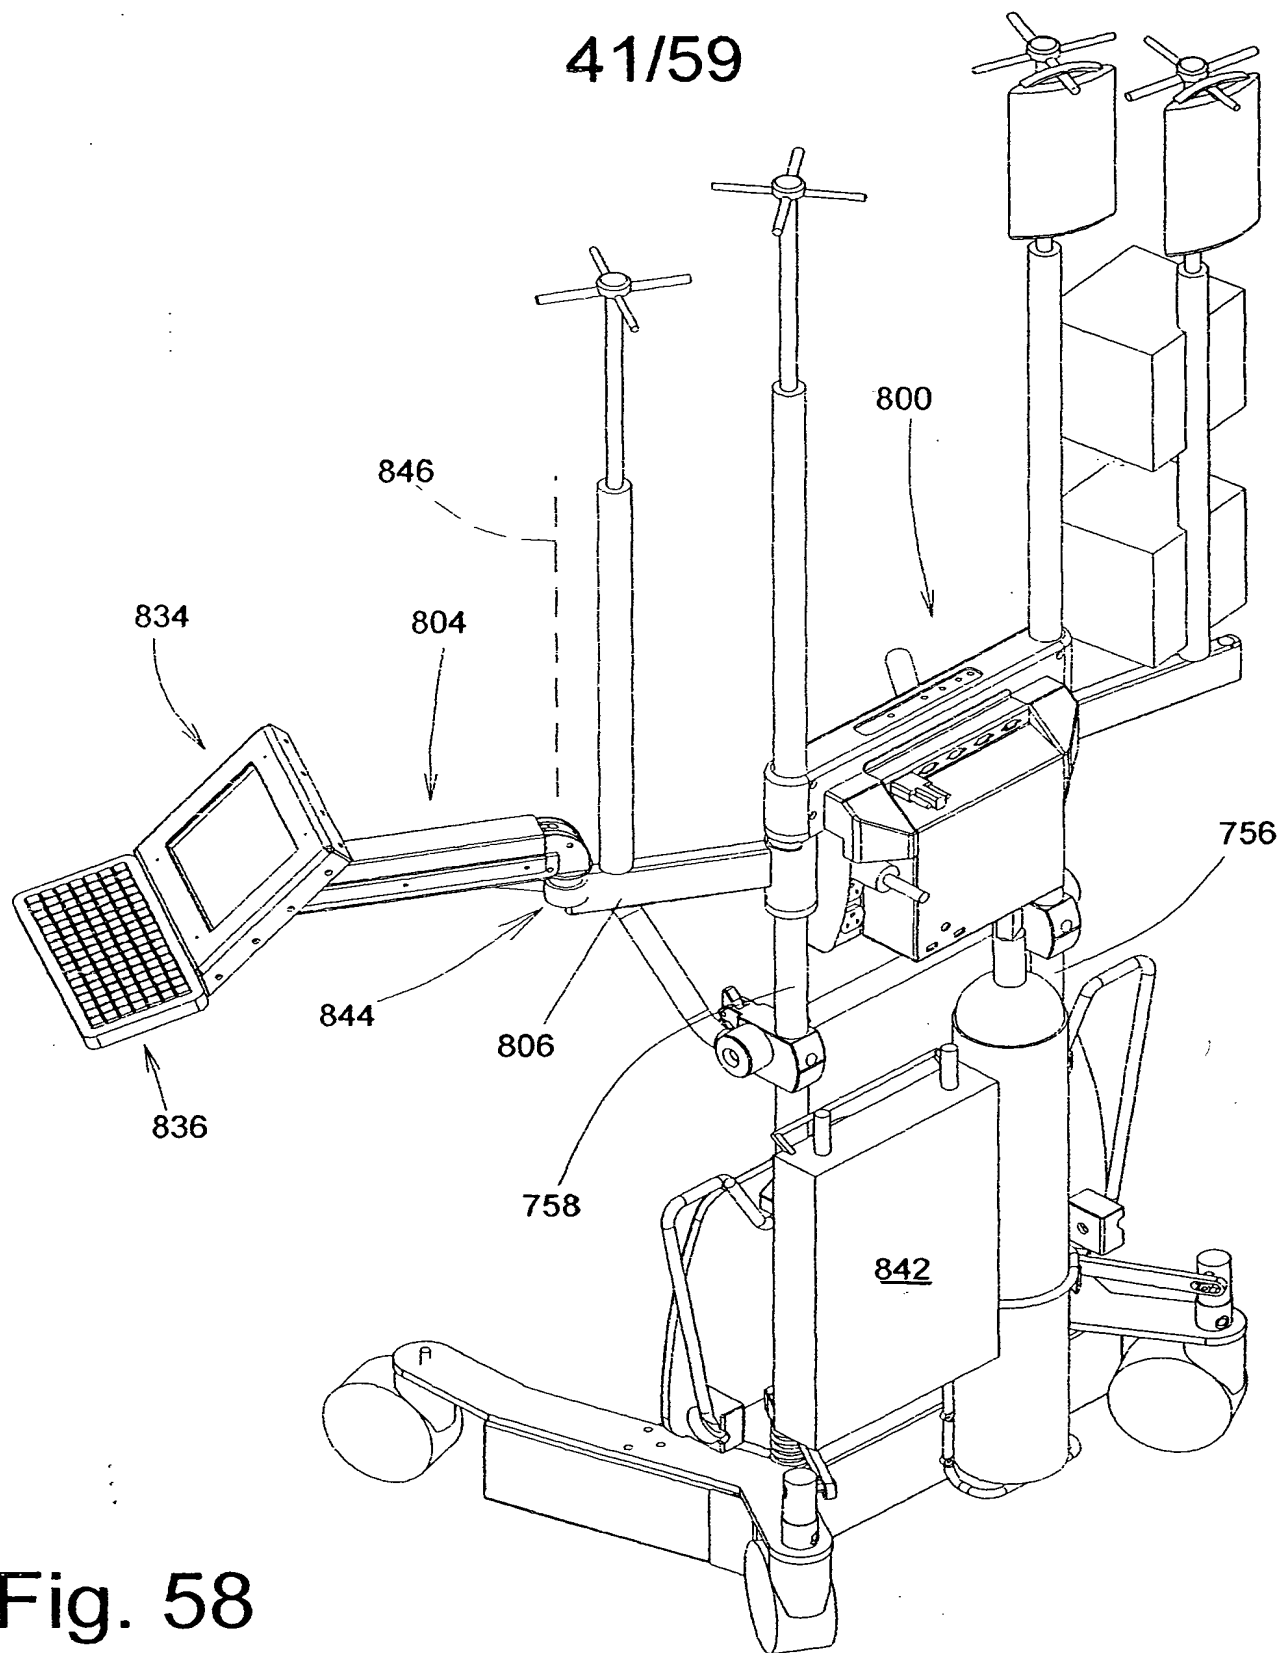


Fig. 58



09849580.121801

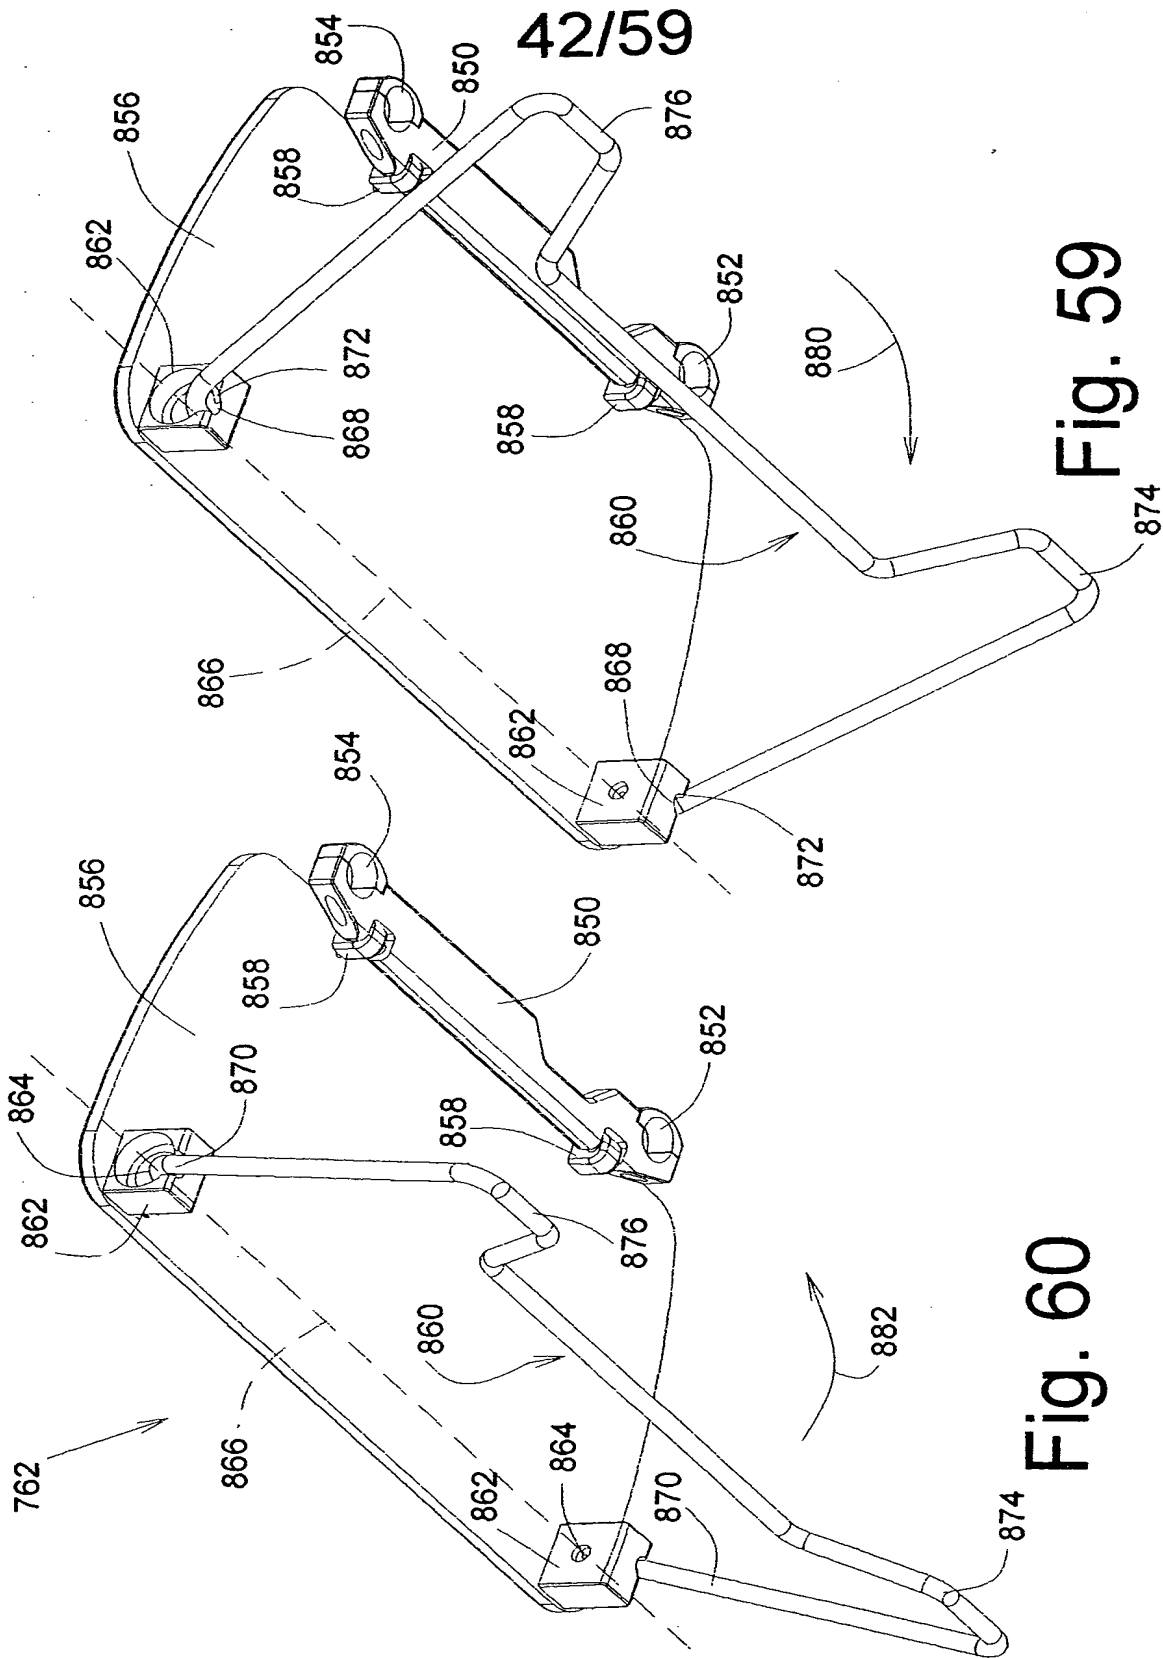

42/59

Fig. 59

Fig. 60

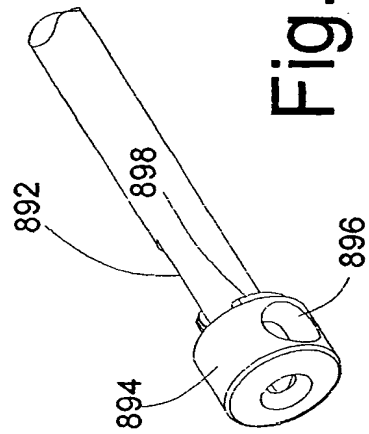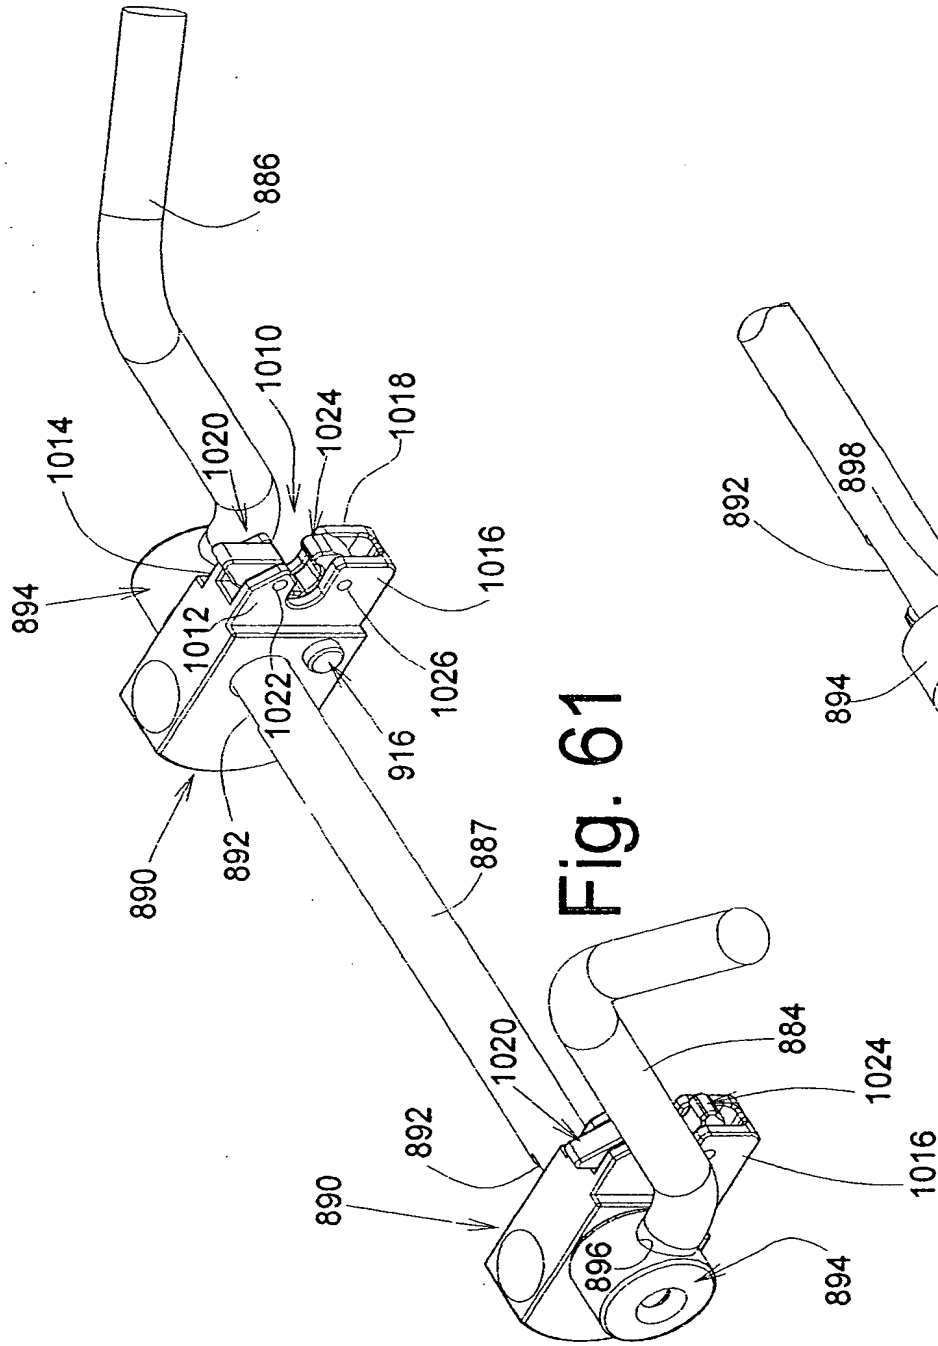

44/59

Fig. 63


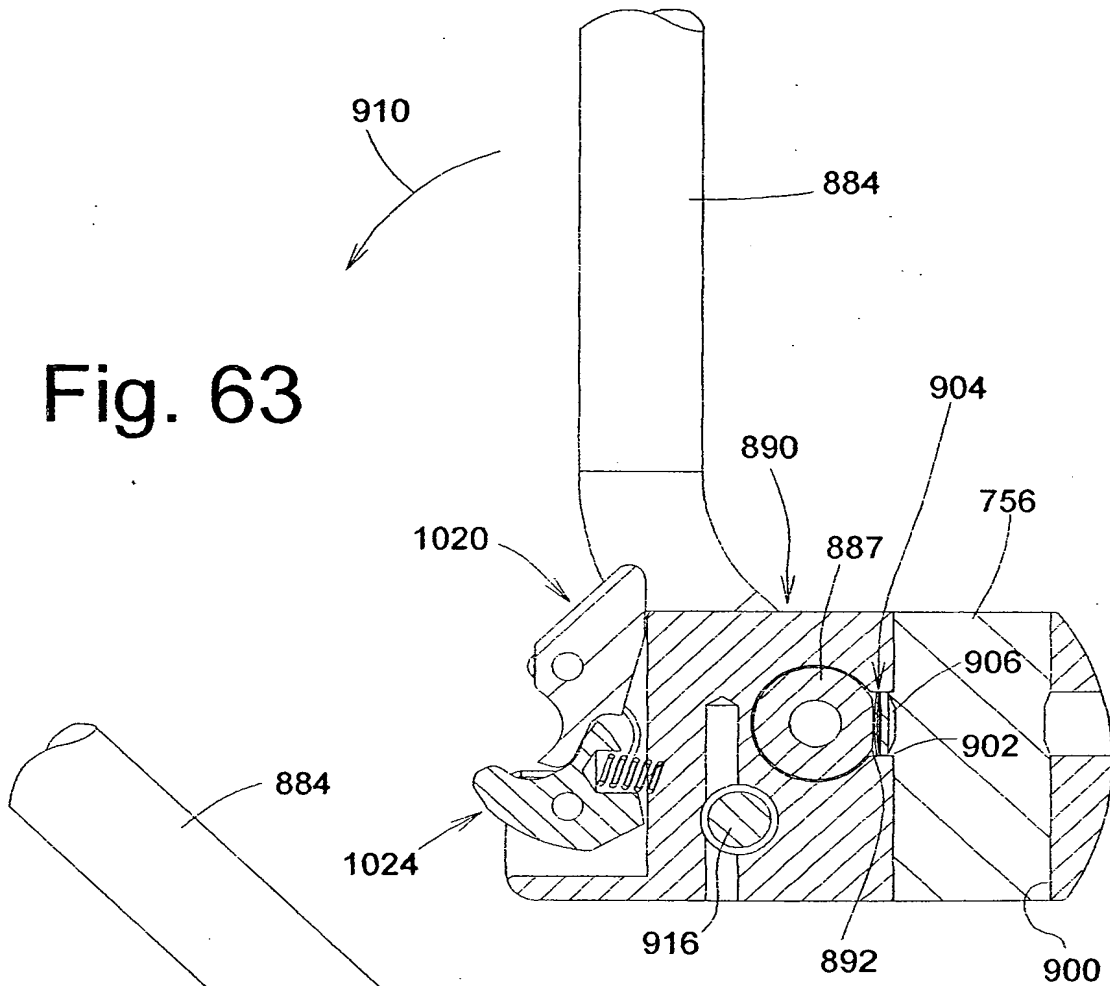


Fig. 64

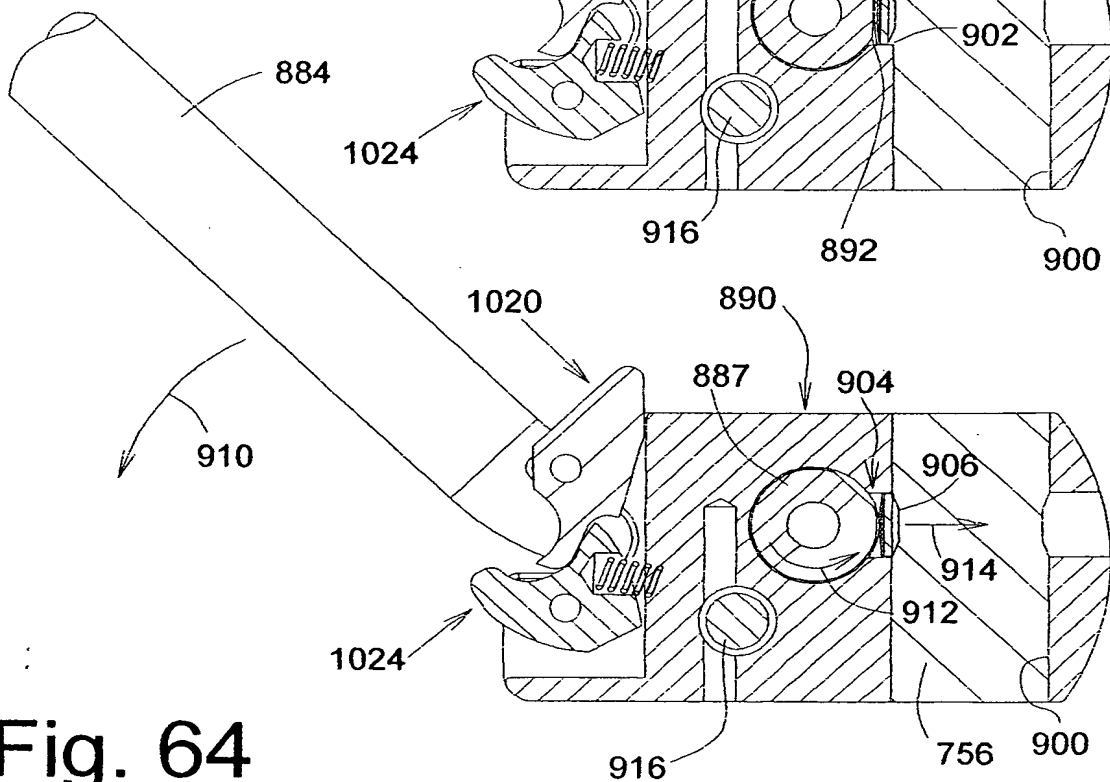

45/59

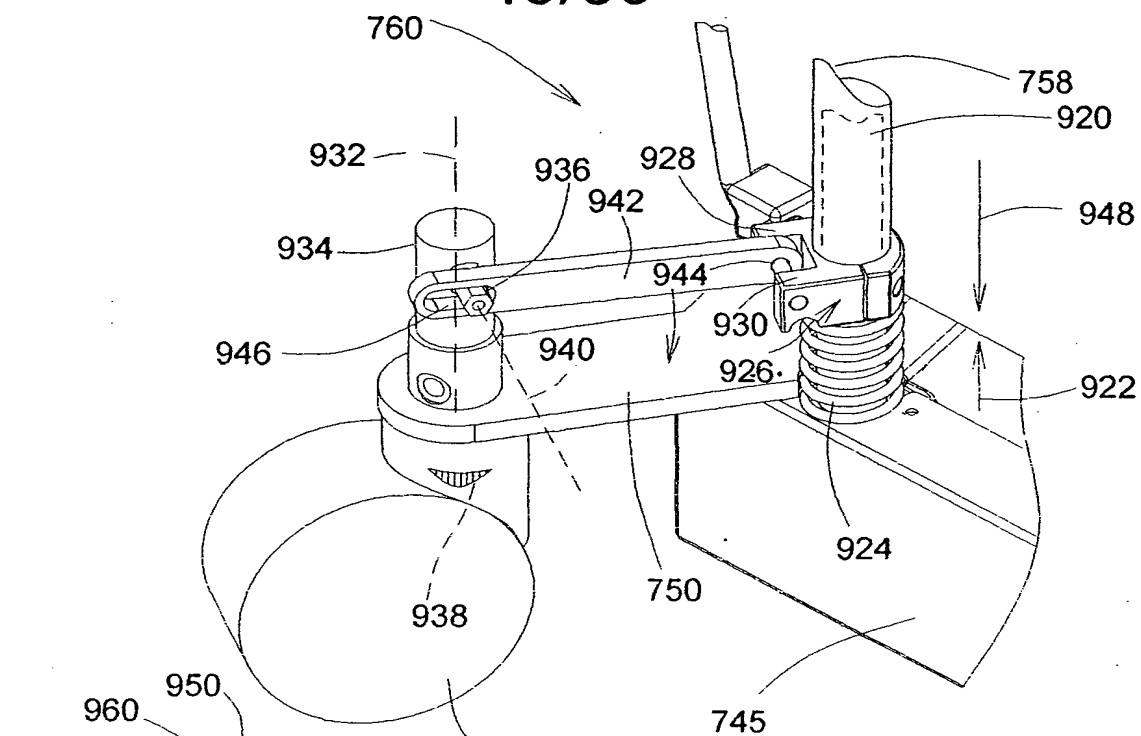


Fig. 65

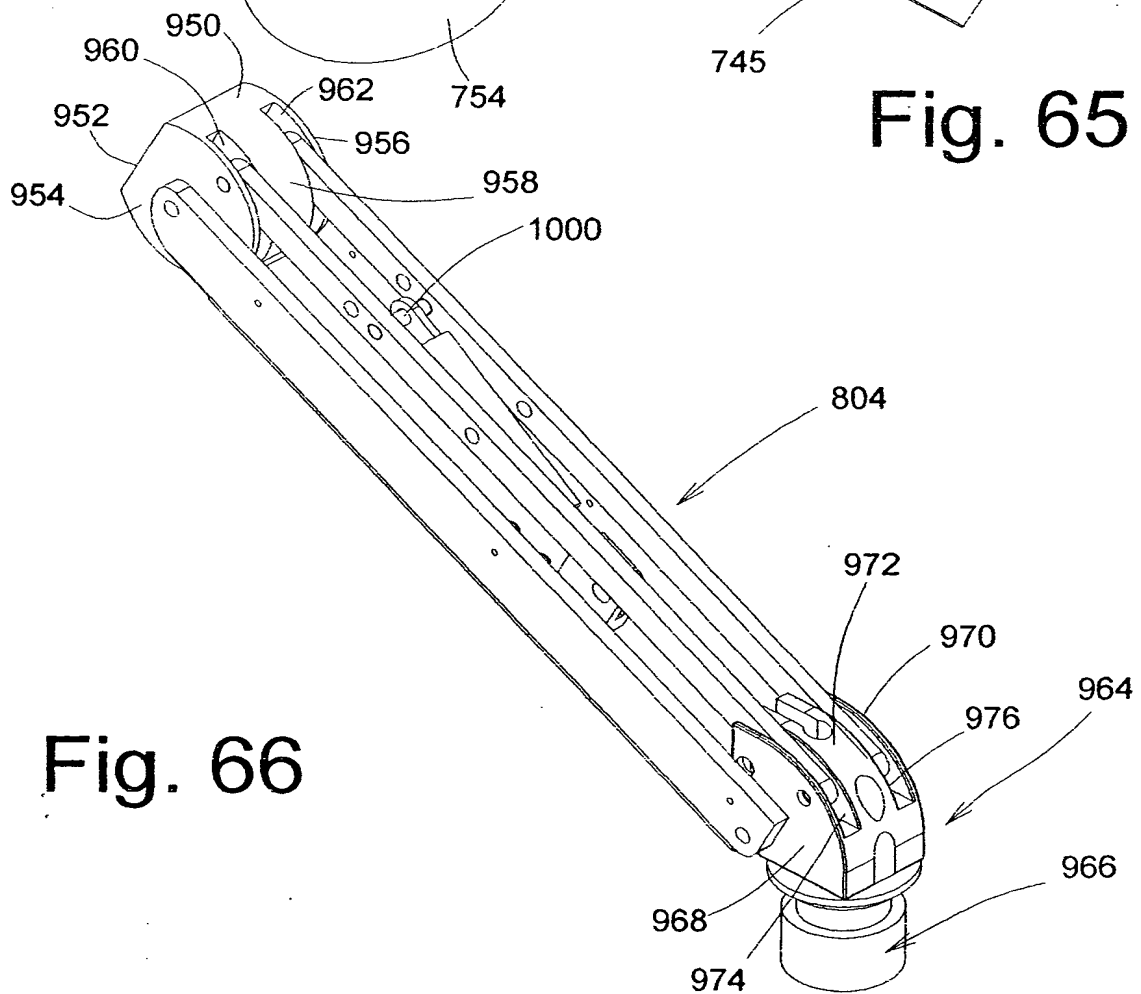


Fig. 66

00849550-121301

46/59

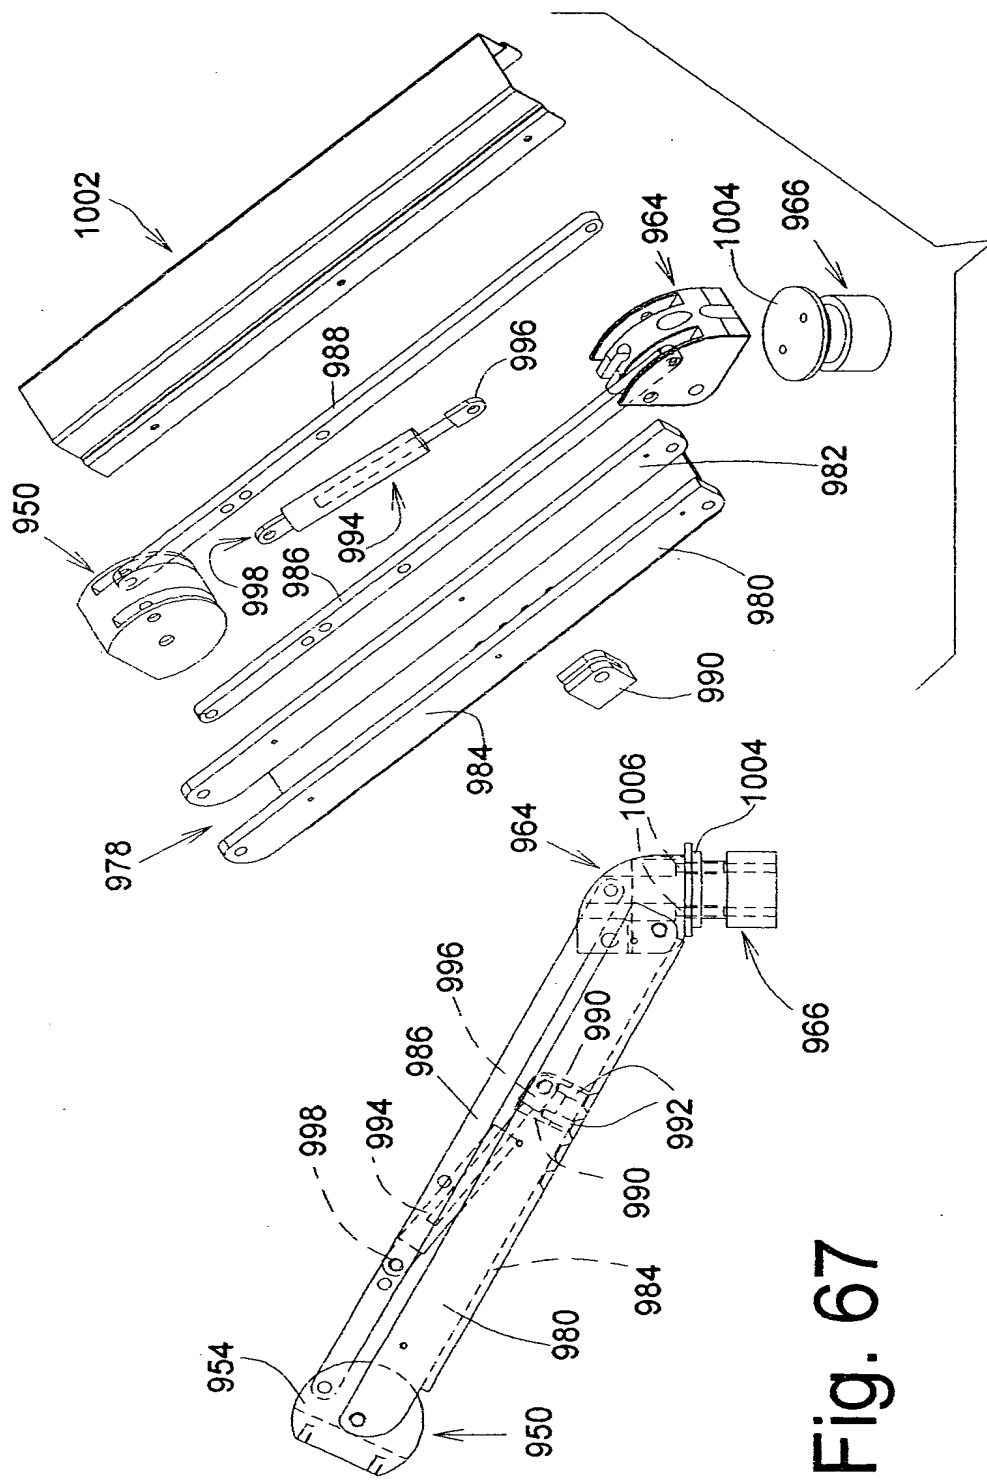


Fig. 67

Fig. 68

47/59

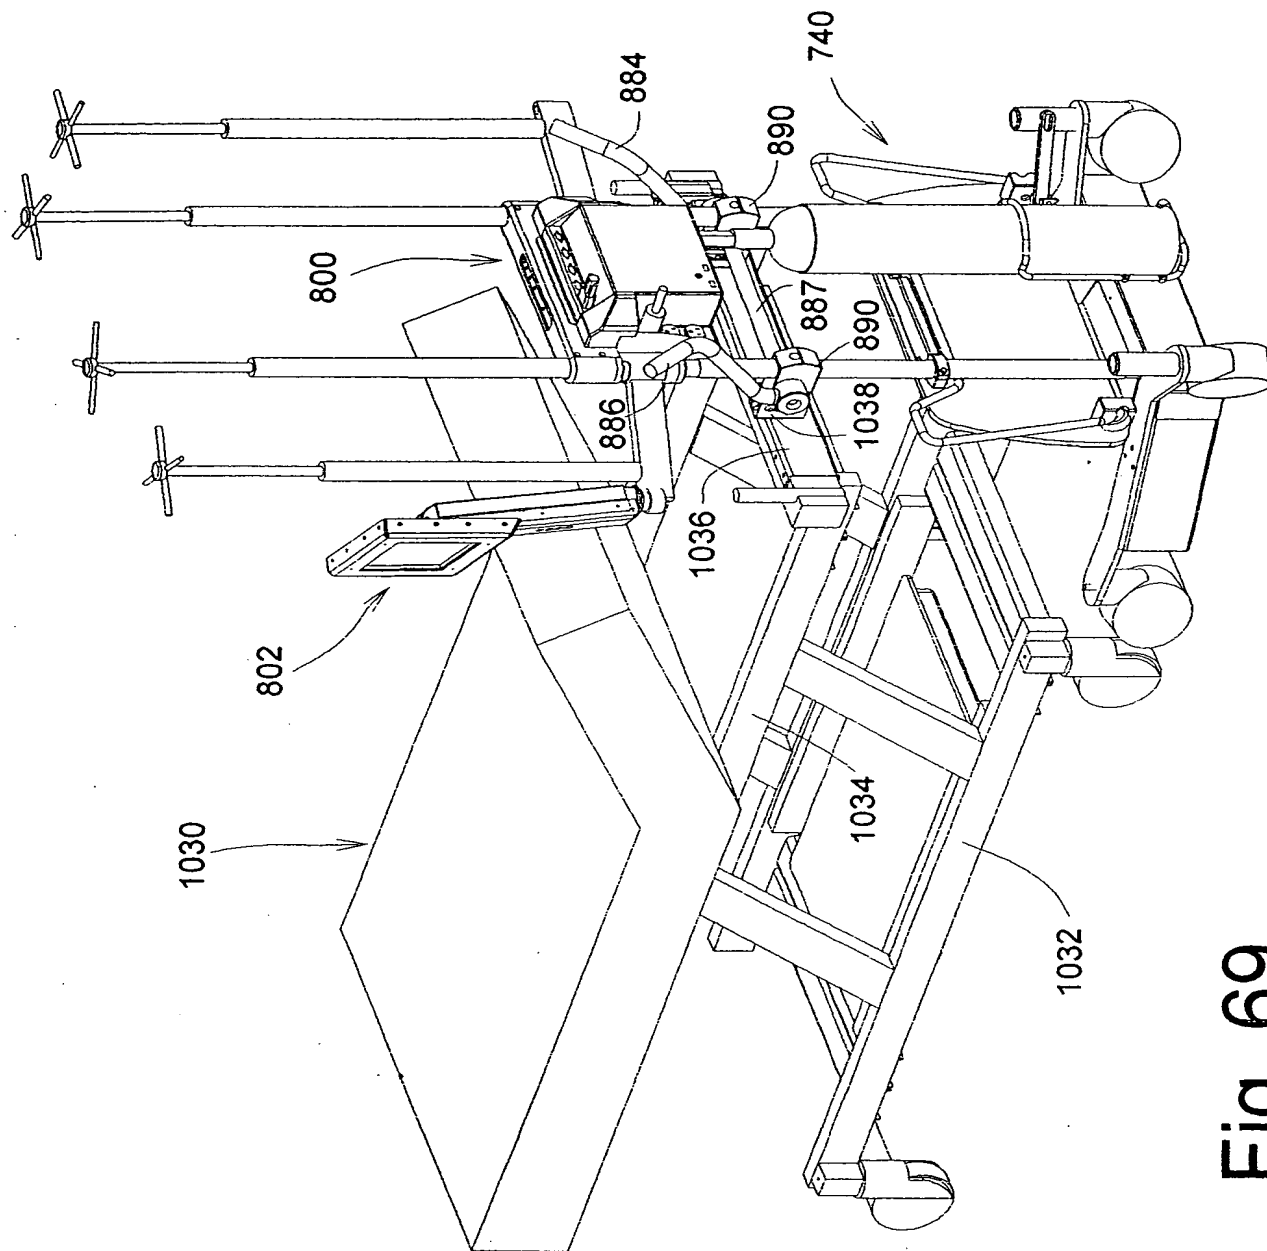


Fig. 69

POSTER 08564860



Fig. 71

Fig. 72

49/59

09849580.121801




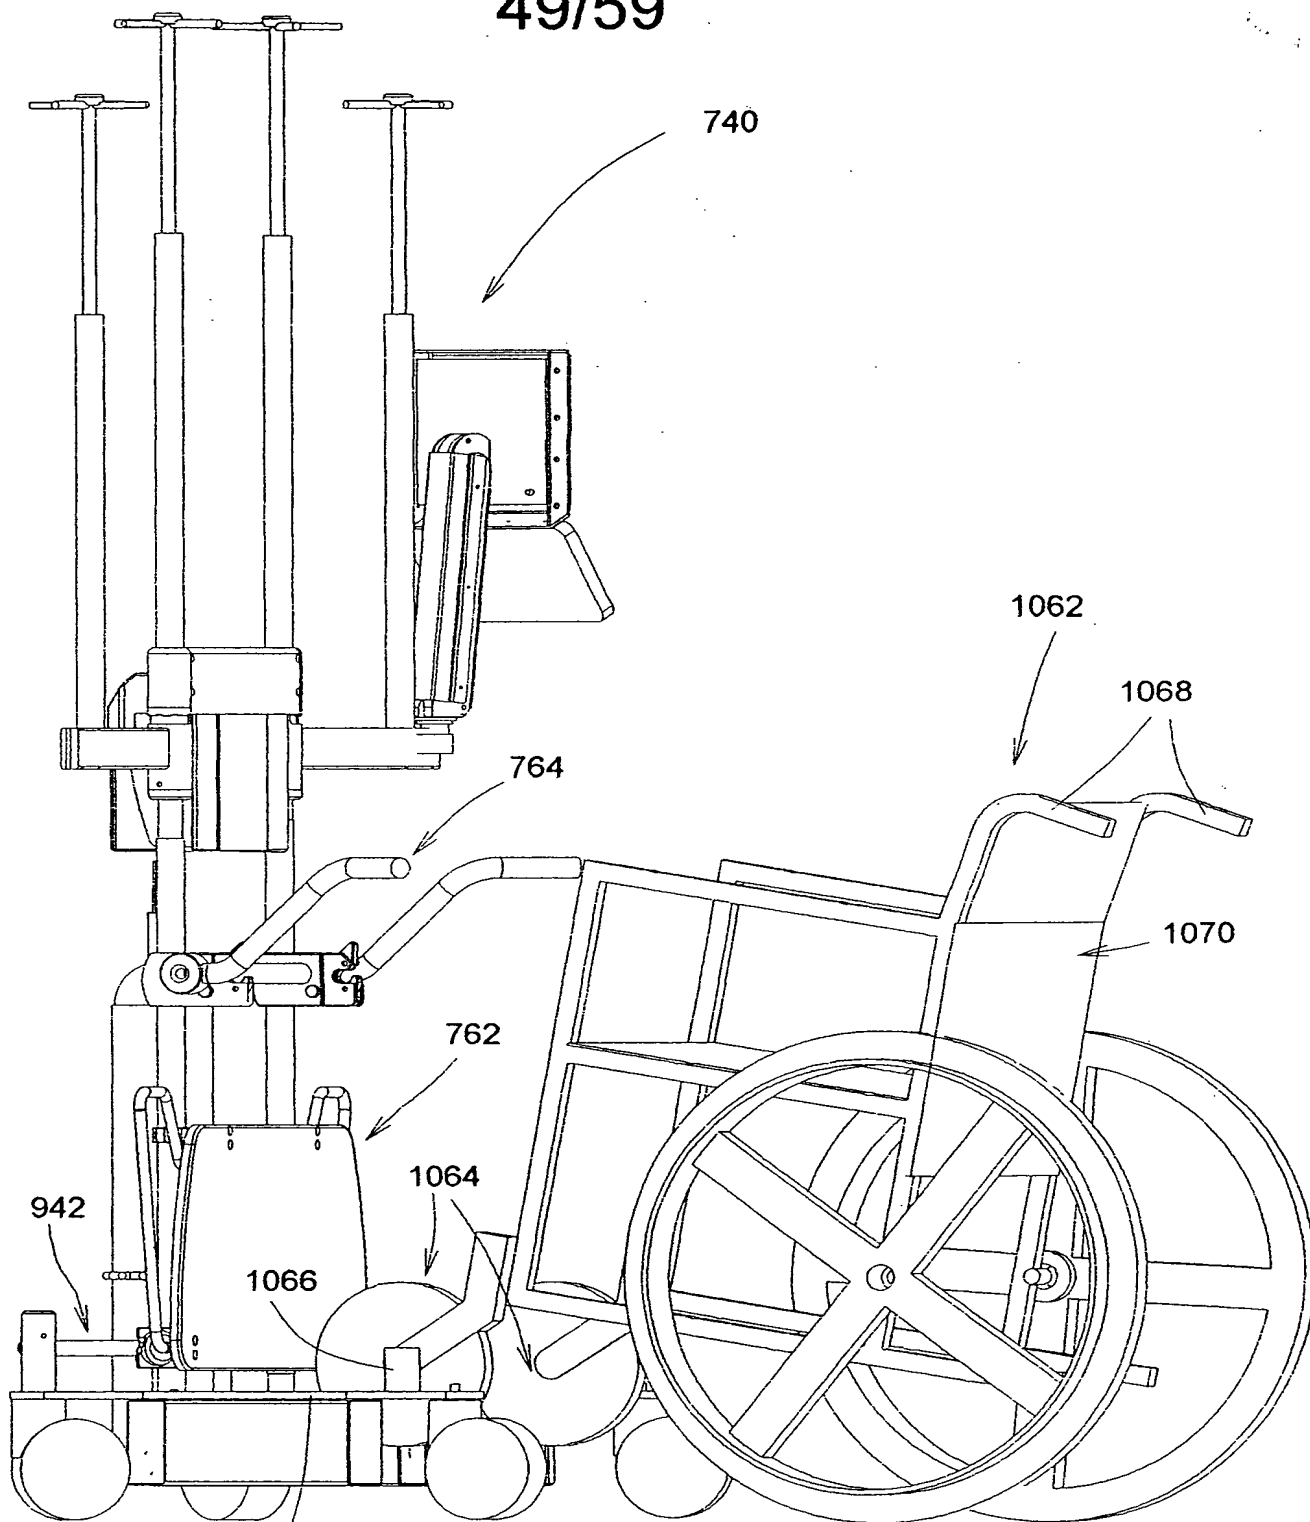


Fig. 73

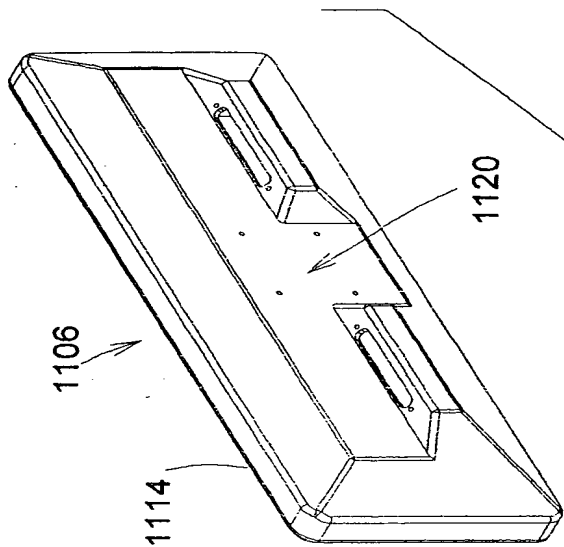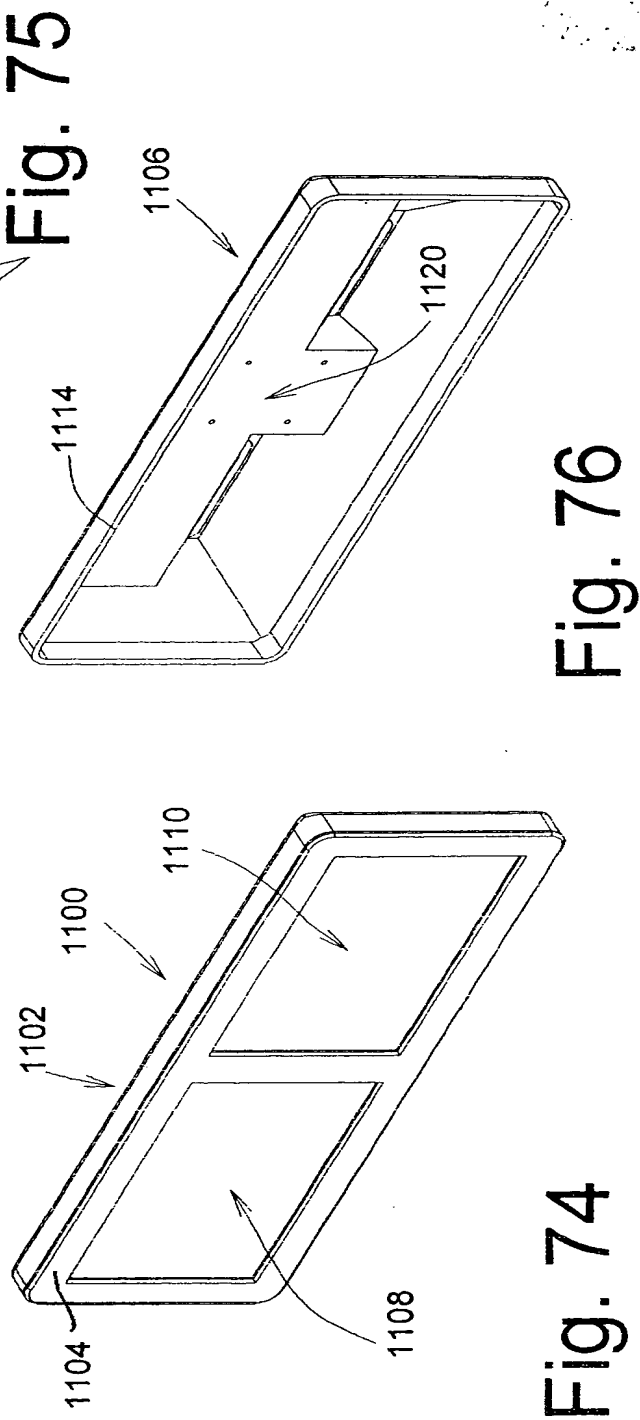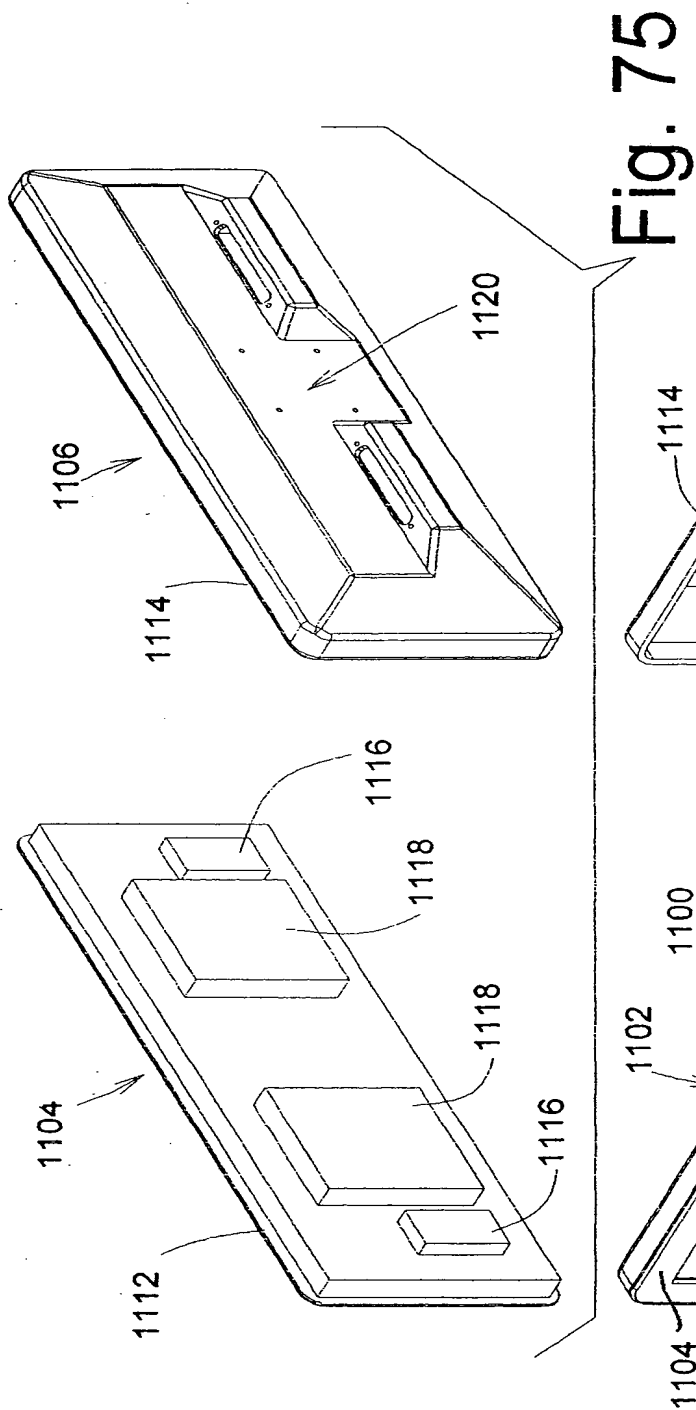

52/59

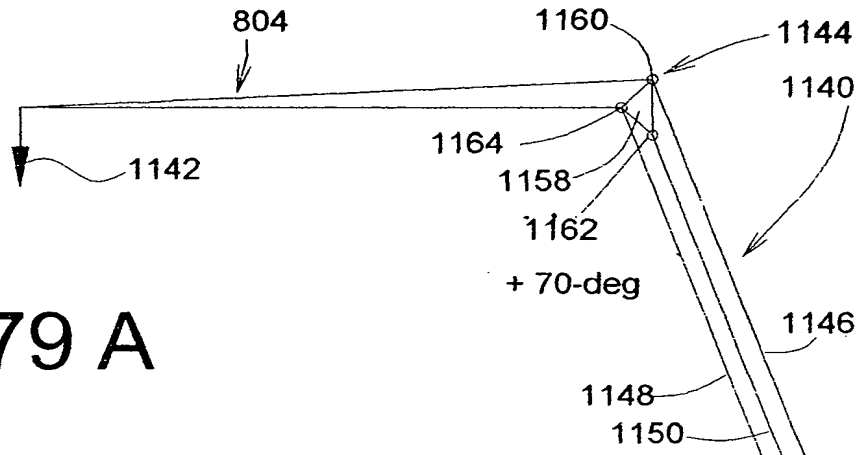


Fig. 79 A

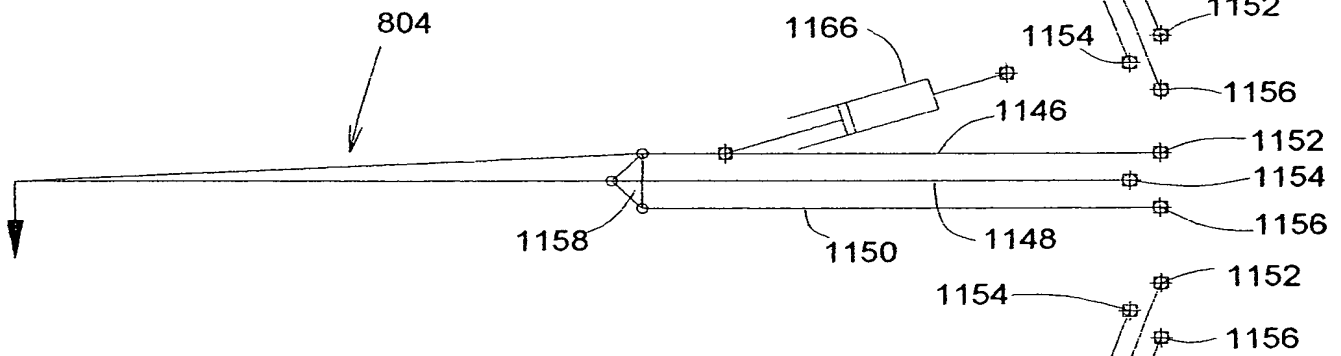


Fig. 79 B

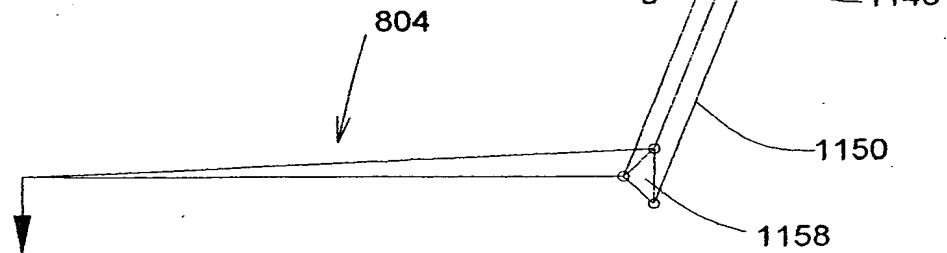


Fig. 79 C

09349580-121801

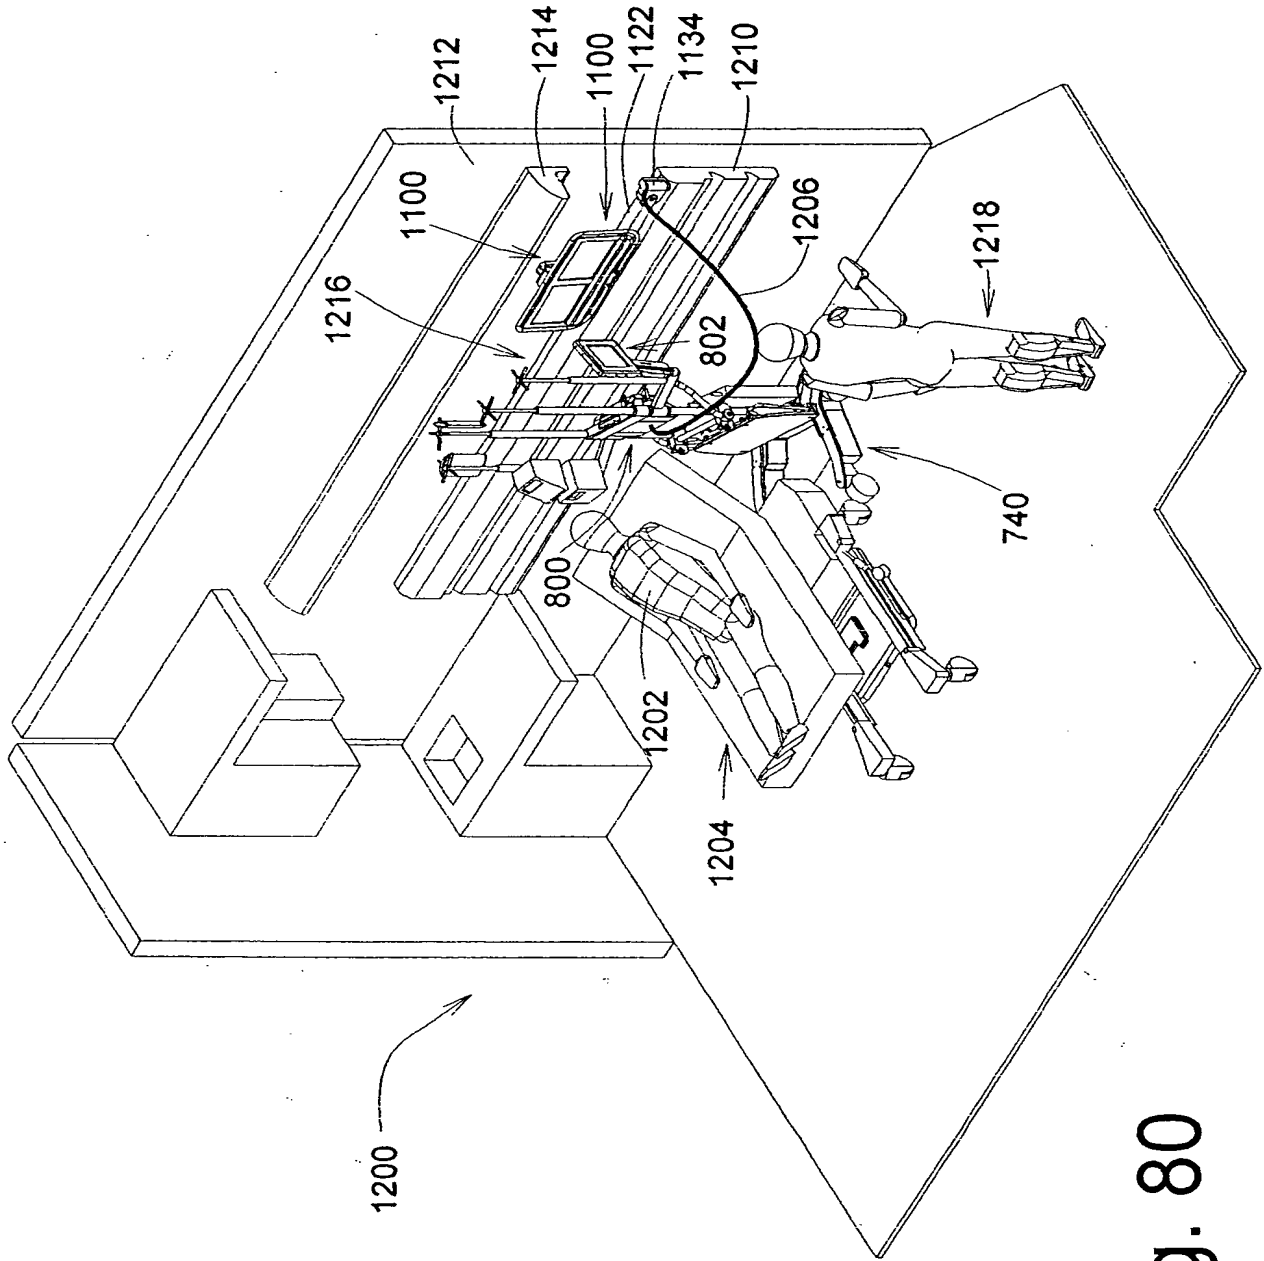


Fig. 80

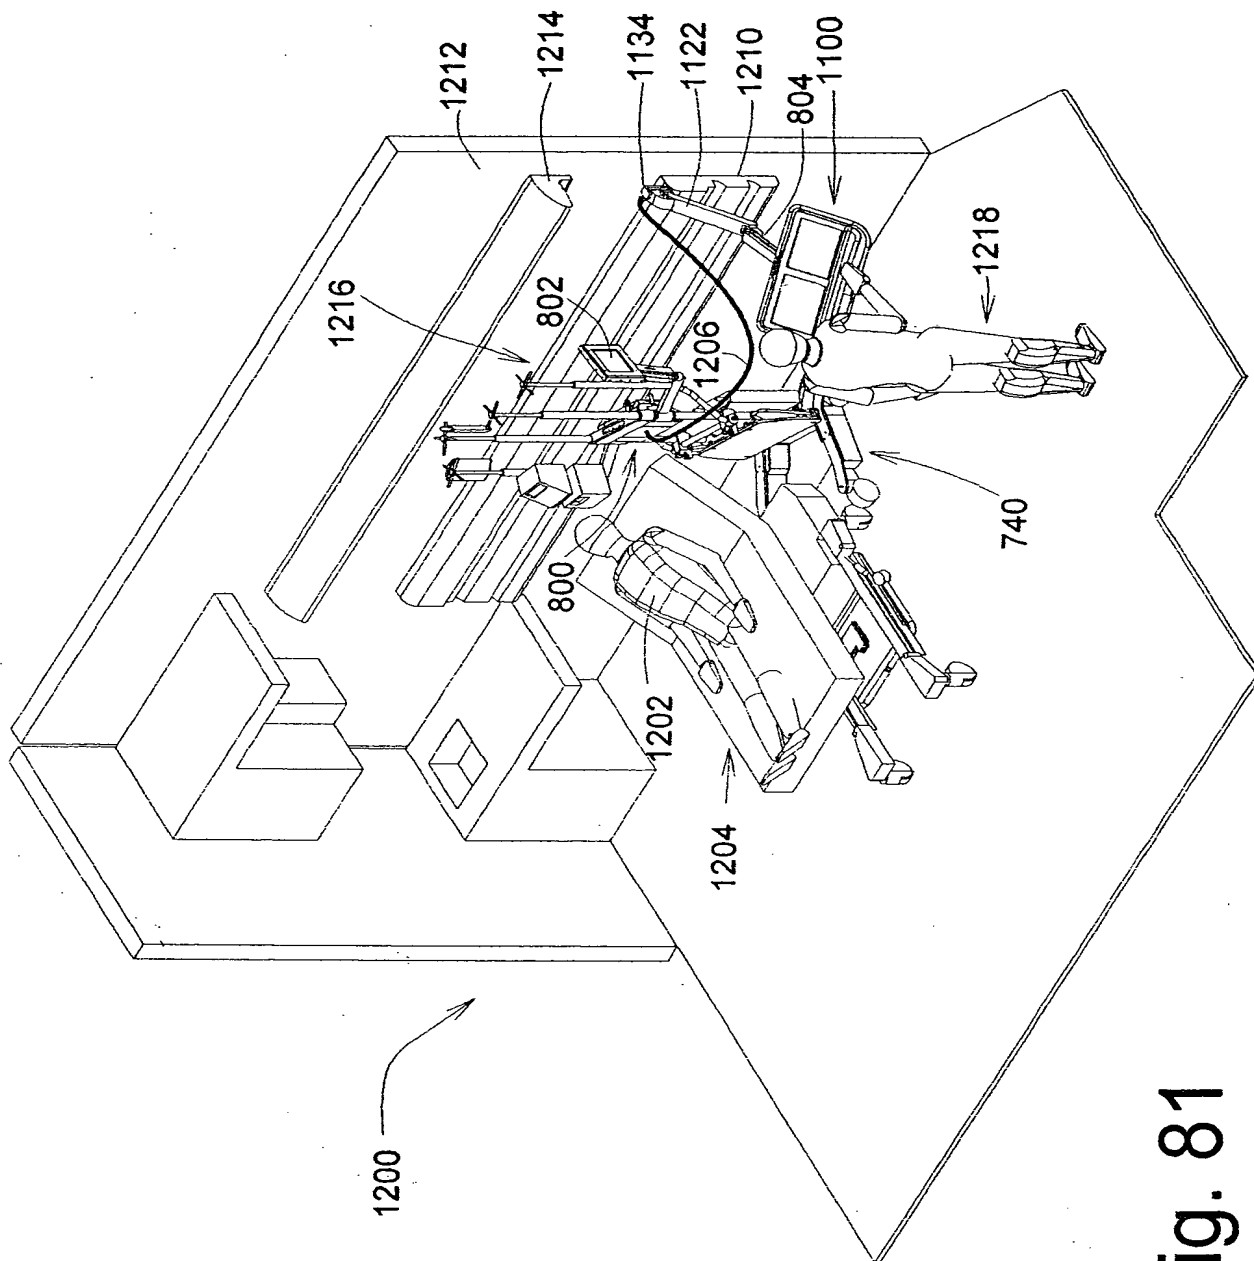


Fig. 81

55/59

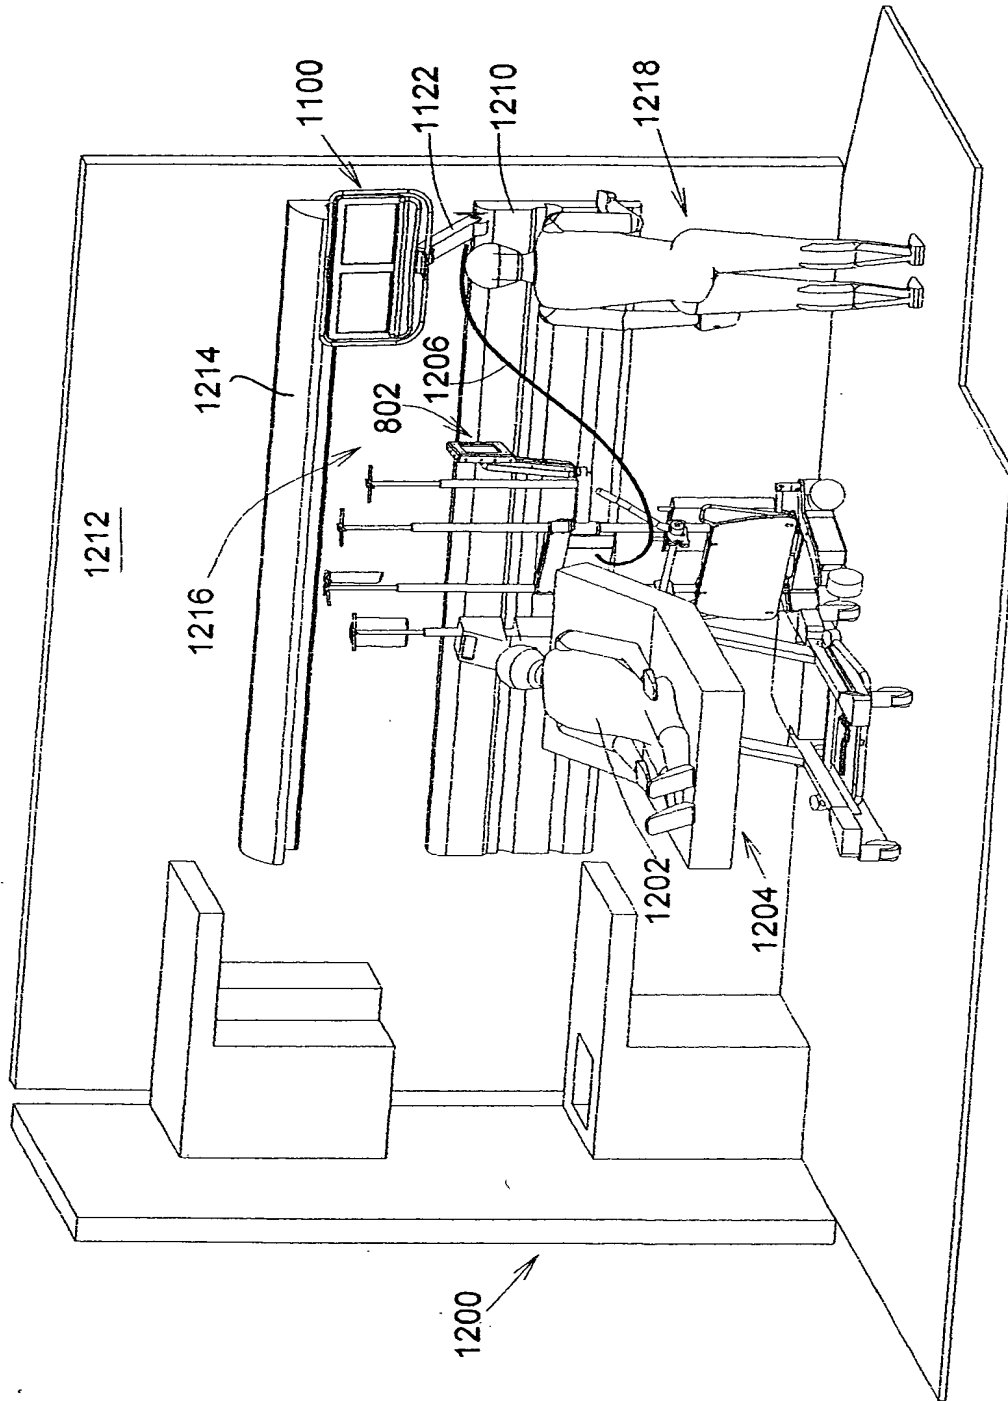


Fig. 82

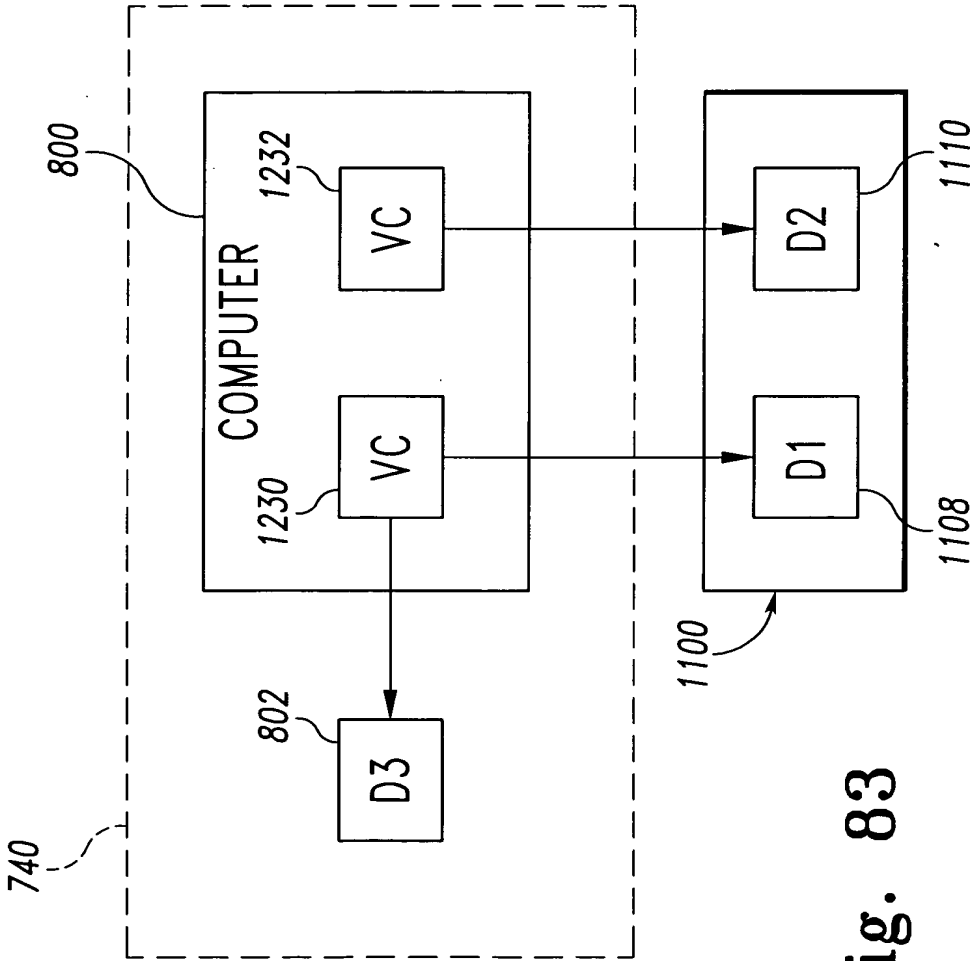


Fig. 83

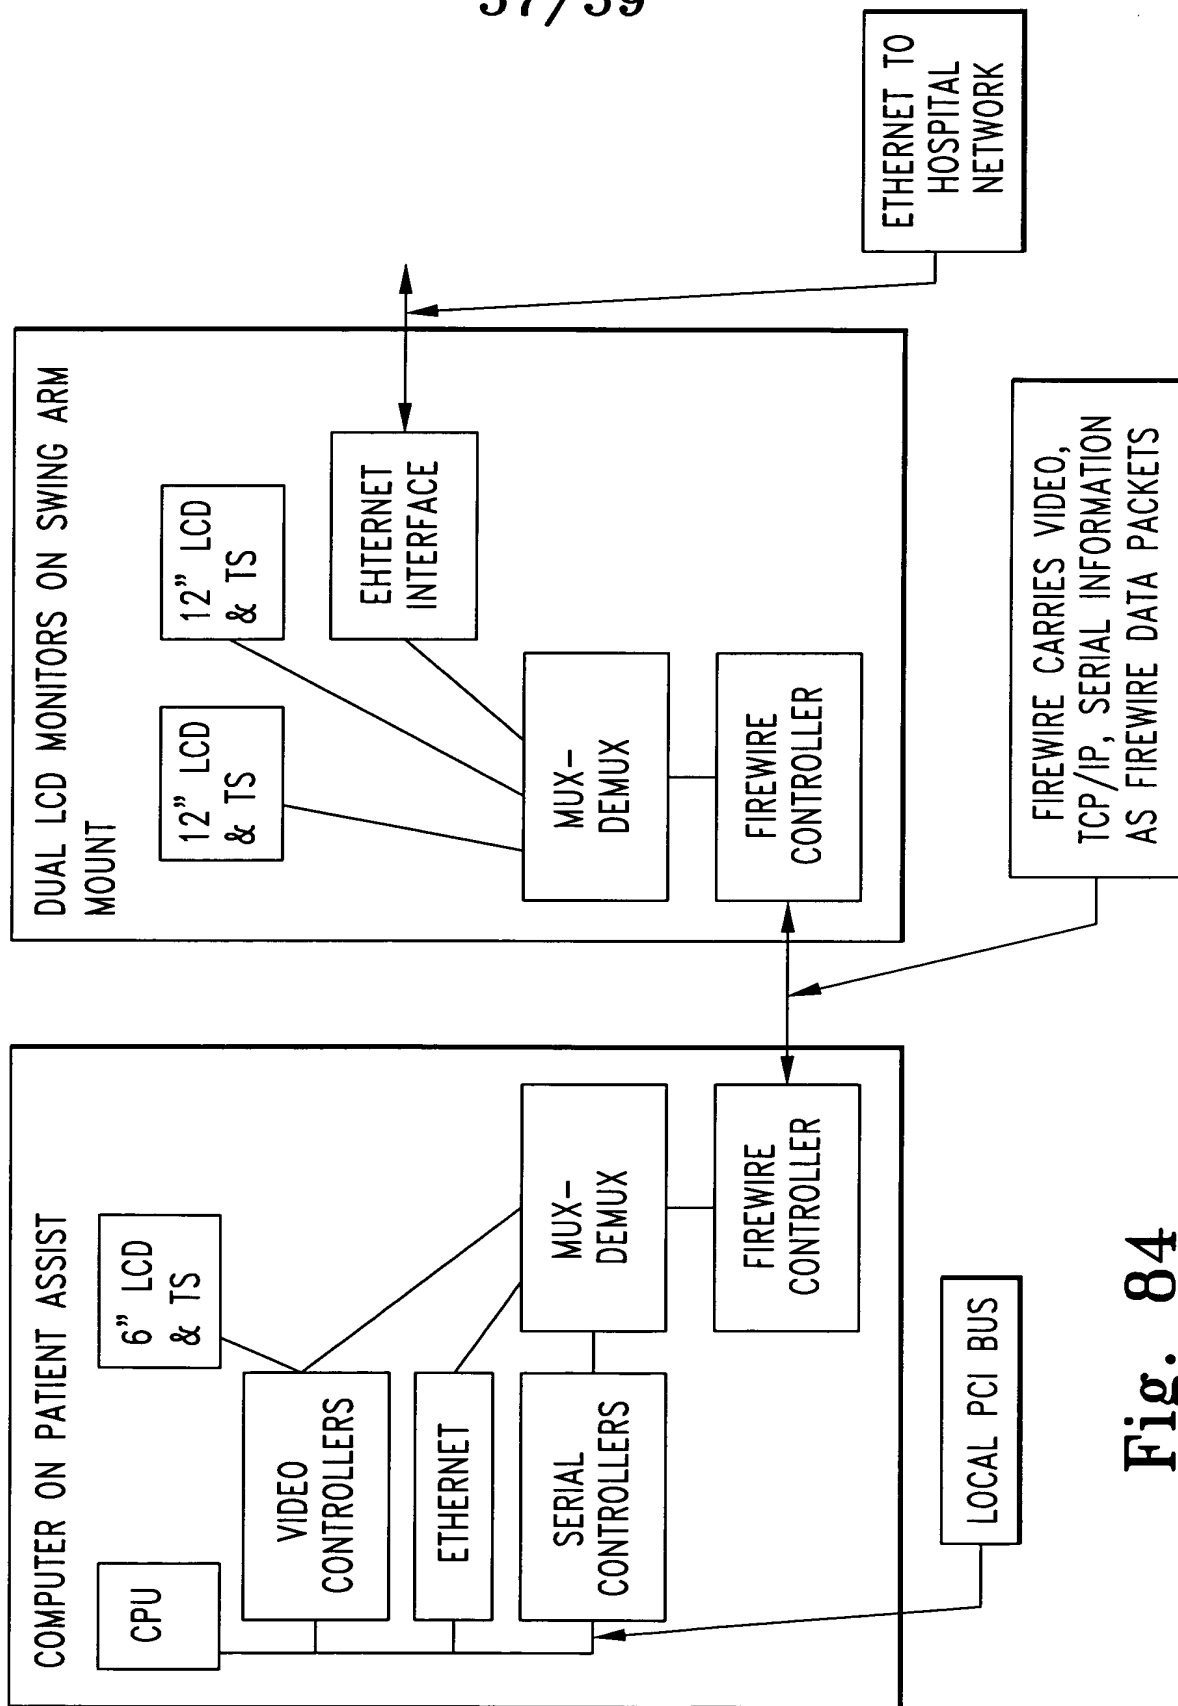


Fig. 84

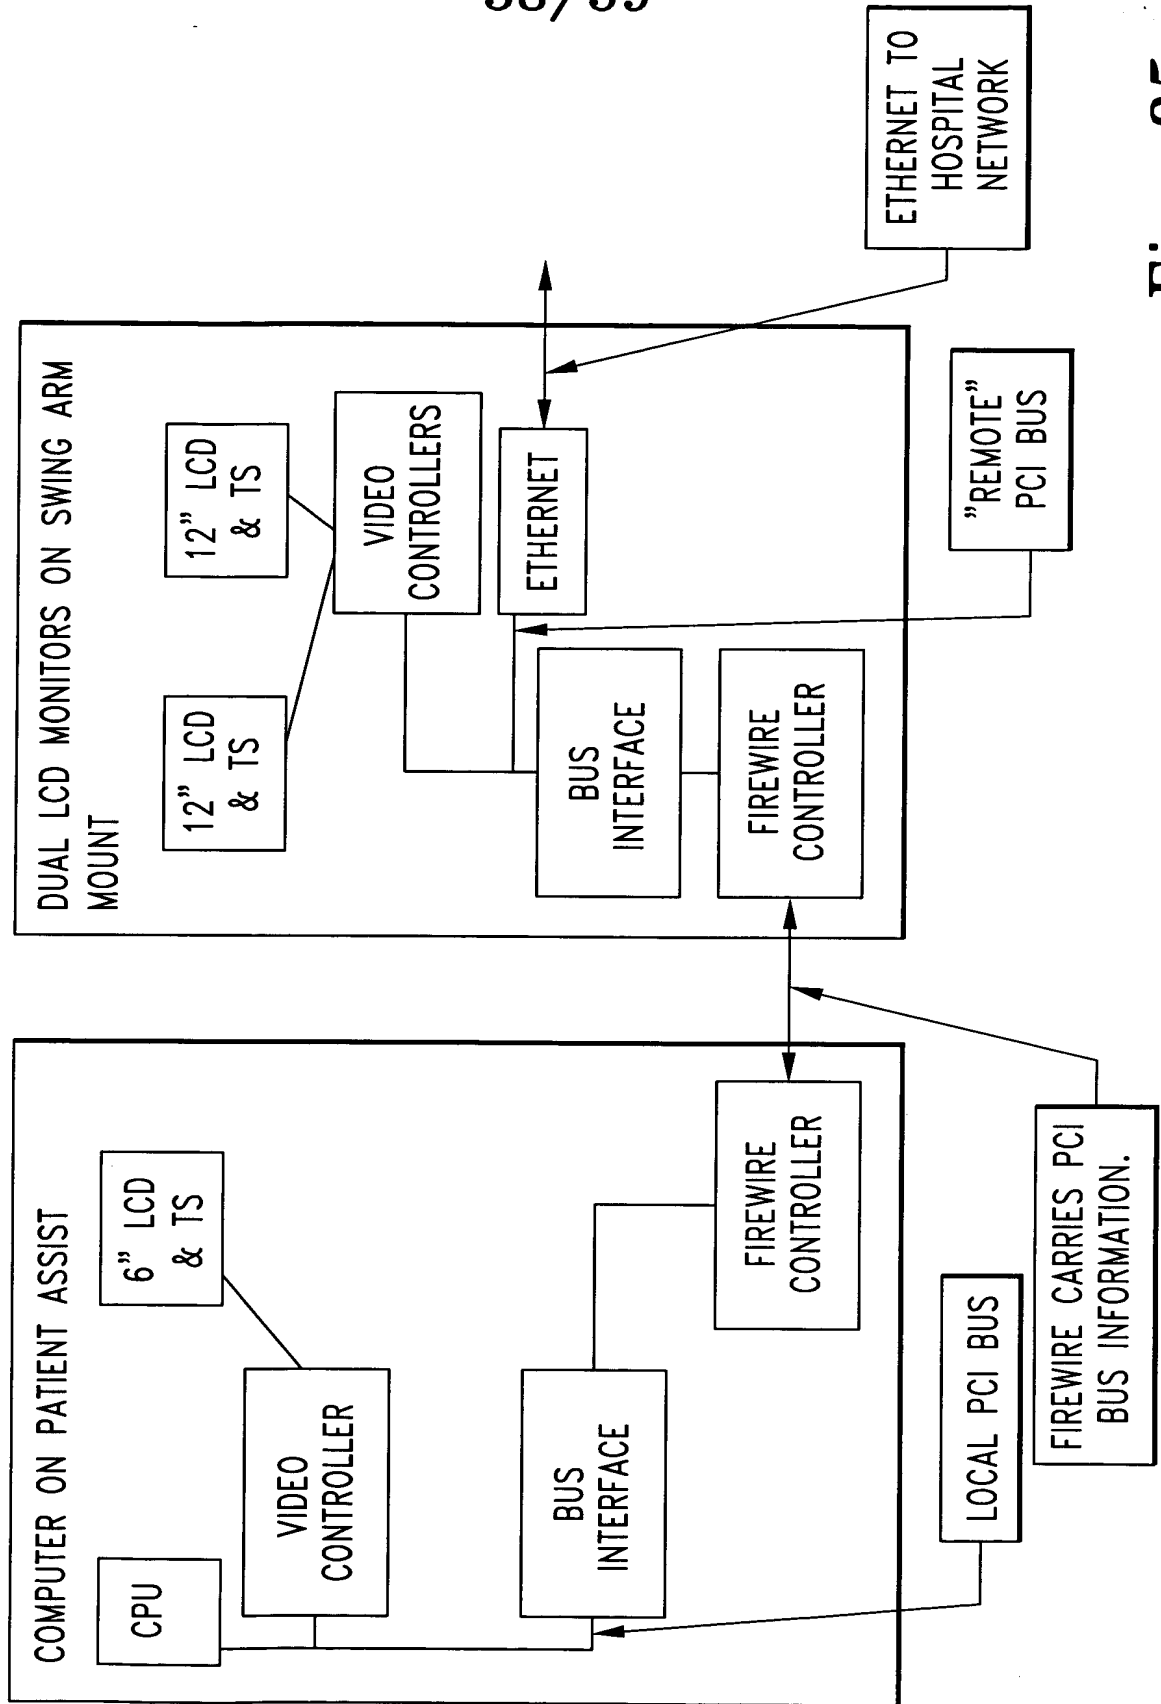


Fig. 85

